



Nalu™ Medical, Inc.

---

## NALU™ NEUROSTIMULATION SYSTEM

### **MAGNETIC RESONANCE IMAGING (MRI) SAFETY INFORMATION**

*It is important to read this entire manual prior to conducting or recommending an MRI examination on a user implanted with the Nalu Neurostimulation System. These instructions only apply to the Nalu Neurostimulation System and do not apply to other products. If you have any questions, please contact Nalu Medical or visit [www.nalumed.com](http://www.nalumed.com).*

# TABLE OF CONTENTS

INTRODUCTION .....	3
HEAD AND EXTREMITY MRI LABELING .....	5
SCS HEAD AND EXTREMITIES SCAN USING A TRANSMIT/RECEIVE HEAD AND EXTREMITIES.....	5
PNS HEAD AND EXTREMITIES SCAN USING A TRANSMIT/RECEIVE HEAD AND EXTREMITIES.....	10
WHOLE-BODY MRI LABELING.....	11
HOW TO DETERMINE THE PATIENT’S WHOLE-BODY MR CONDITIONALITY .....	11
DEVICE CONFIGURATIONS.....	13
NERVE TARGET.....	14
SINGLE LEAD LOOK-UP TABLE .....	24
DUAL LEAD LOOK-UP TABLE .....	29
LABELS .....	46
APPENDIX A .....	172
WHOLE-BODY MRI QUICK REFERENCE GUIDE .....	172
CONTACT INFORMATION .....	173

# INTRODUCTION

*The following information applies to all MR Conditional labels contained in this manual.*

**All the components of the Nalu Neurostimulation System are MR Unsafe except for the following:**

- *Nalu Implantable Pulse Generator Dual 4 Ported (Model 11007-002) connected to one or two 25 cm Nalu Tined Leads (Model 12005-025)*
- *Nalu Implantable Pulse Generator Dual 4 Ported (Model 11007-002) connected to one or two 40 cm Nalu Tined Leads (Model 12005-040)*
- *Nalu Implantable Pulse Generator Dual 4 Ported (Model 11007-002) connected to one 25 cm Nalu Tined Leads (Model 12005-025) and one 40 cm Nalu Tined Leads (Model 12005-040)*
- *Nalu Implantable Pulse Generator Dual 8 Ported (Model 11004-002) connected to one or two 40 cm Nalu Multilumen Leads (Model 12001-040)*
- *Nalu Implantable Pulse Generator Dual 8 Integrated, 40 cm (Model 11002-040)*
- *Nalu Implantable Pulse Generator Alternate Pitch Dual 8 Ported (Model 11009-002) connected to one or two 40 cm Nalu Alternate Pitch Leads (Model 12010-040)*
- *Nalu Implantable Pulse Generator Single 4 Ported (Model 11006-002) connected to a 25 cm Nalu Tined Lead Model (12005-025)*
- *Nalu Implantable Pulse Generator Single 4 Integrated, 25 cm Tined (Model 11005-025)*
- *Nalu Implantable Pulse Generator Single 4 Ported (Model 11006-002) connected to a 40 cm Nalu Tined Lead (Model 12005-040)*
- *Nalu Implantable Pulse Generator Single 4 Integrated, 40 cm Tined (Model 11005-040)*
- *Nalu Implantable Pulse Generator Single 8 Ported (Model 11003-002) connected to a 40 cm Nalu Multilumen Lead (Model 12001-040)*
- *Nalu Implantable Pulse Generator Single 8 Integrated, 40 cm (Model 11001-040)*
- *Nalu Anchor (Model 13001).*

## **WARNING**

**Do not bring MR Unsafe components of the Nalu Neurostimulation System into the MRI system room.**

### **Additional conditions for all MRI Examinations**

- Do not perform MRI if the patient has a device or device component lead(s), extension, etc. attached to the Nalu Implantable Pulse Generator or leads from a different manufacturer attached to the Nalu Implantable Pulse Generator. The risk of performing an MRI examination under those circumstances has not been evaluated and, thus, may cause harm to the patient and/or the components.
- Nalu Neurostimulation System external components are not allowed in MRI system room. These components include Therapy Discs (Model 34001 or Model 34002), the iOS™ or Android™ device with the Nalu Remote Control application, Charger, Clinician Programmer and Belts, surgical instruments or accessories. All such parts are **MR Unsafe** and are not permitted in the MRI system room.
- Do not perform MRI on a patient undergoing the trial phase of the Nalu Implantable Pulse Generator (i.e., the patient has a percutaneously implanted lead and an external Trial Therapy Disc (Model 34002).

- Do not perform MRI on a patient that has any other active medical implants.

### **Preparation of the Patient Prior to the MRI Examination**

- Inform the patient of the risks associated with undergoing an MRI examination: an MRI exam performed outside recommended guidelines may result in the electromagnetic fields used with MRI technology interacting adversely with an implanted Nalu Neurostimulation System, potentially injuring the patient and/or damaging the device.
- A trained healthcare professional with the proper knowledge of MRI technology such as an MRI safety-trained radiologist, MRI technologist, MRI nurse, or MRI physicist must ensure that the MRI examination will be conducted according to the information presented in this document.
- Perform an impedance check. Do not perform an MRI if the impedance is greater than 10 k $\Omega$ .
- Remove the Therapy Disc from the patient before entering the MRI system room.
- Do not conduct an MRI examination if the implanted lead(s) are not connected to the Nalu Implantable Pulse Generator.
- Do not sedate or anesthetize the patient so that the patient can inform the MRI system operator of any unusual sensations or problems associated with the MRI examination.
- Instruct the patient to immediately inform the MRI system operator if any discomfort, stimulation, shocking, or heating is experienced during MRI.

### **Additional Preparation of Patients with more than one Nalu Neurostimulation System**

- If the patient has more than one implanted Nalu Neurostimulation System, there must be a minimum distance of 50 mm between any part of the systems (IPG and lead(s)). Do not perform an MRI examination on a patient if there is less than 50 mm between the implanted systems.
- If the Nalu Neurostimulation Systems are implanted in different body regions, it can be assumed that there is at least 50 mm between the systems. The body regions, as referred to above, are defined as the head, neck, torso, upper extremities, and lower extremities.
- If the Nalu Neurostimulation Systems are implanted in the same body region, the distance between the systems must be confirmed before the MRI examination. The distance should be confirmed through imaging, such as fluoroscopy or X-Ray.

### **Considerations during the MRI Examination**


- Similar to other MRI examinations, carefully monitor the patient throughout the MRI procedure both visually and audibly. Immediately discontinue the MRI examination if the patient reports any problems or unusual sensations.

### **Considerations after the MRI Examination**

- After the patient leaves the MRI system room, turn the Therapy Disc on and verify connection to the Implantable Pulse Generator.
- Perform an impedance check.

# HEAD AND EXTREMITY MRI LABELING

## SCS Head and Extremities scan using a transmit/receive head and extremities


MR Conditional	
	
<b>MRI Safety Information</b> For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury.	
Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T or 3.0 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Head and Extremity
Receive Coil Type	Head and Extremity
RF Conditions	First Level Controlled - Partial body SAR of the exposed body part of 10 W/kg and Head SAR of 3.2 W/kg
Scan Duration	Scan for up to 15 minutes.
Scan Regions	<p>For head/brain MRI examinations, only the transmit/receive RF head coil is permitted for use. No parts of the implanted Nalu Neurostimulation System may be within the transmit/receive RF head coil.</p> <p>For extremity MRI examinations, only use a transmit/receive RF coil that includes a knee, foot/ankle, or wrist transmit/receive RF coil. No part of the implanted Nalu Neurostimulation System may be within one of these transmit/receive RF coils.</p>
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may result in the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

Acceptable 1.5 T/64-MHz or 3 T/128 MHz MRI Scenarios


**Note the position of the implantable pulse generator (IPG) and leads relative to the transmitted RF energy for each respective transmit/receive RF coil.**

*Head/Brain MRI Examination*

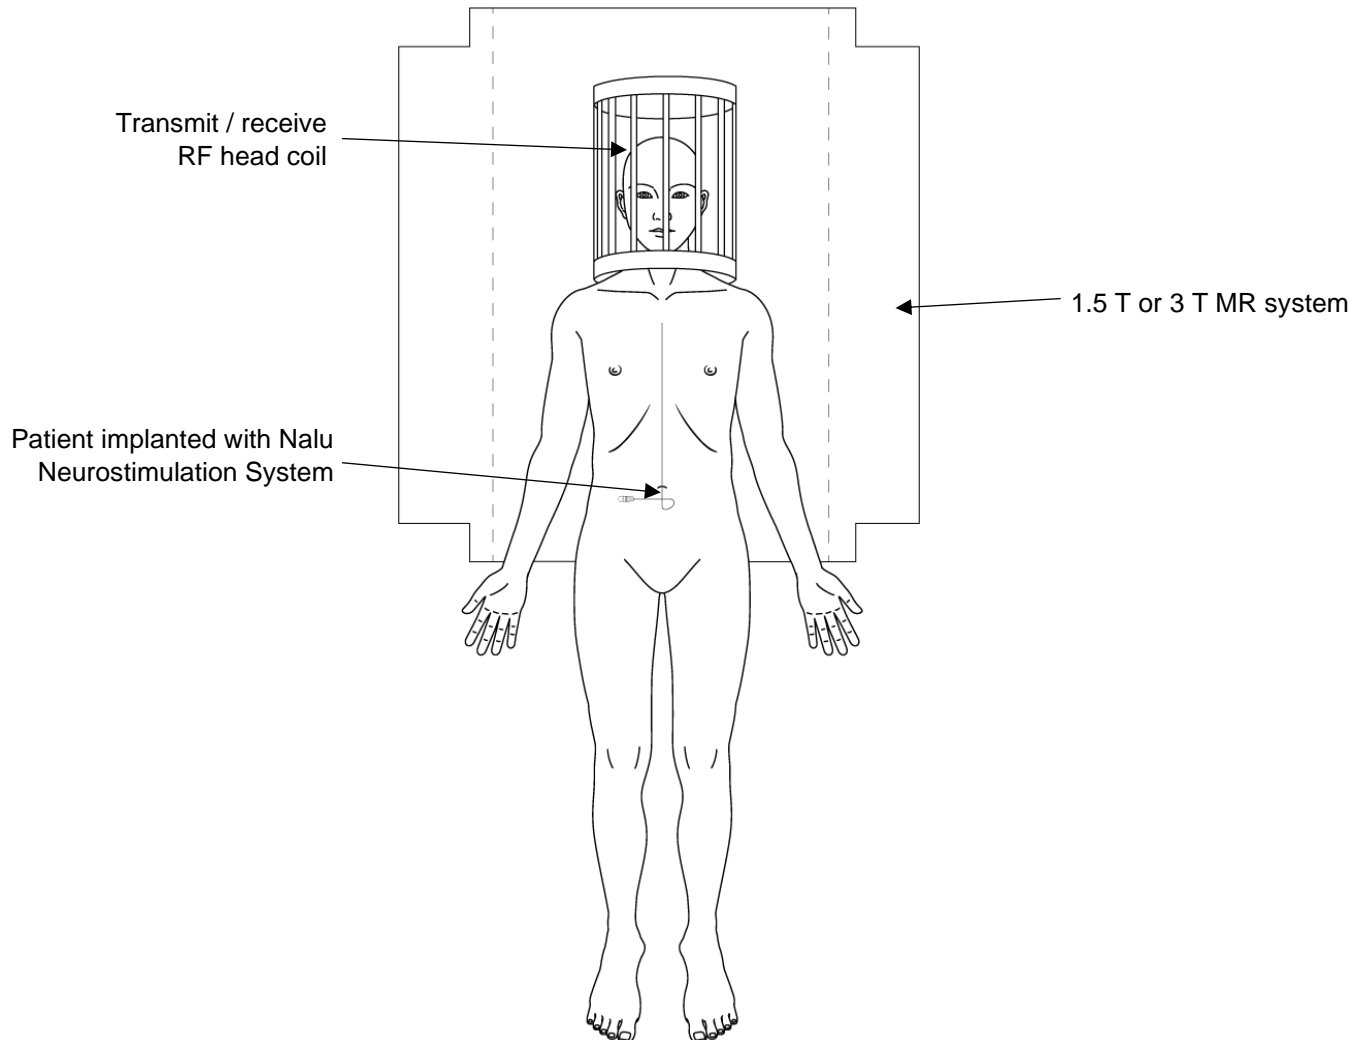


**Figure 1.** Head/brain MRI examinations are permitted using a 1.5 T or 3 T MRI system and a transmit/receive RF head coil. No part of the implanted Nalu Neurostimulation System may be within the transmit/receive RF head coil. All other aforementioned conditions must be carefully followed.

## Extremity MRI Examinations

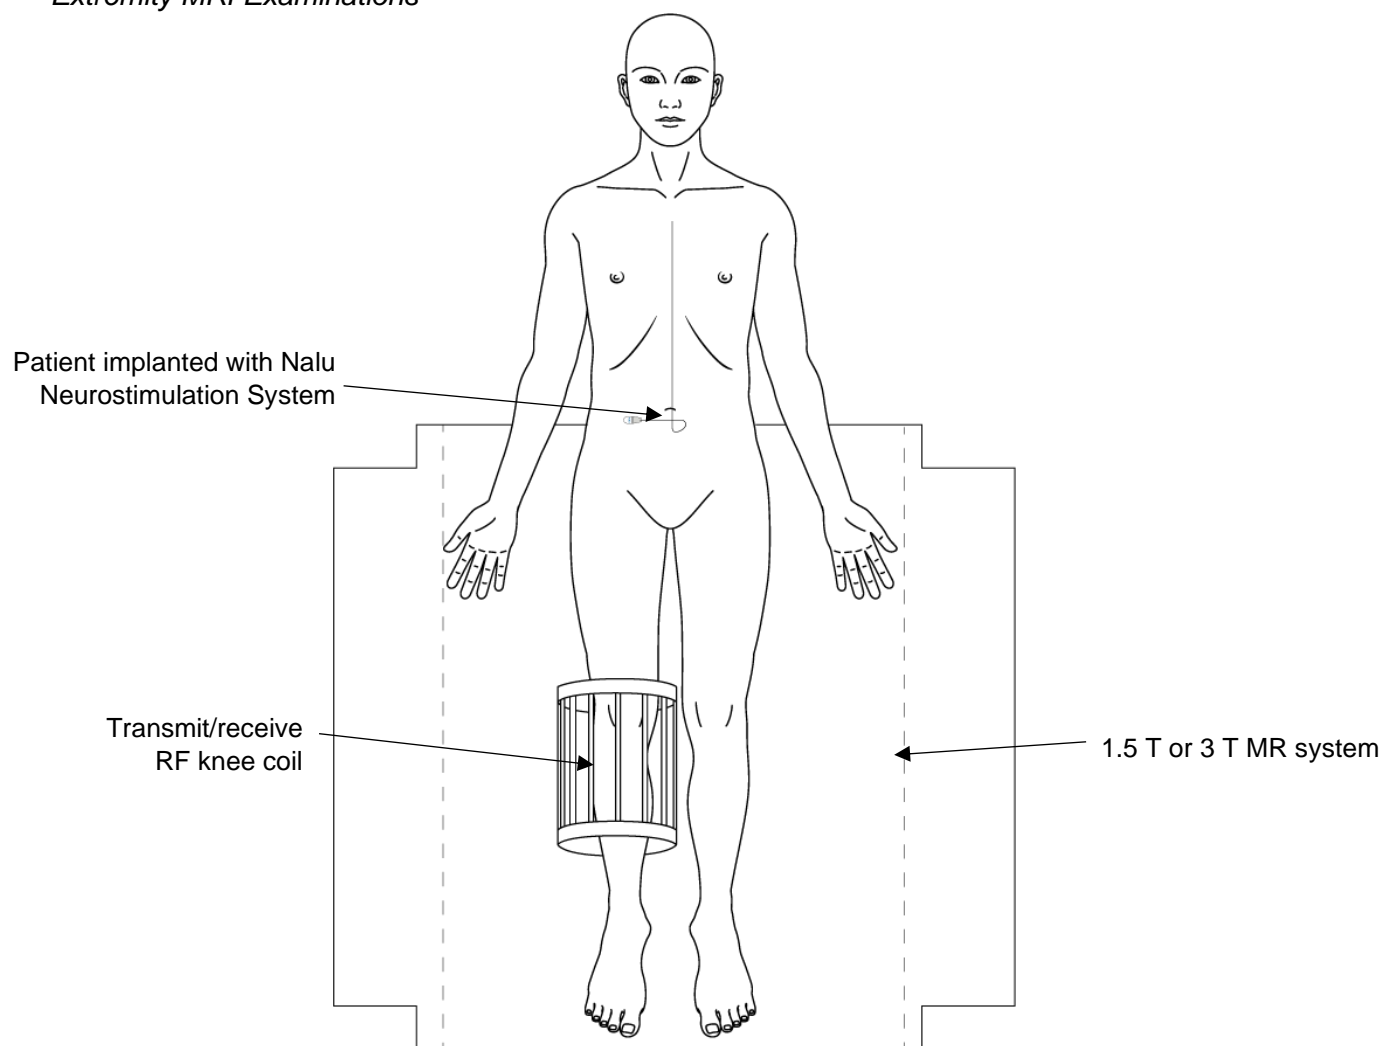


**Figure 2a**

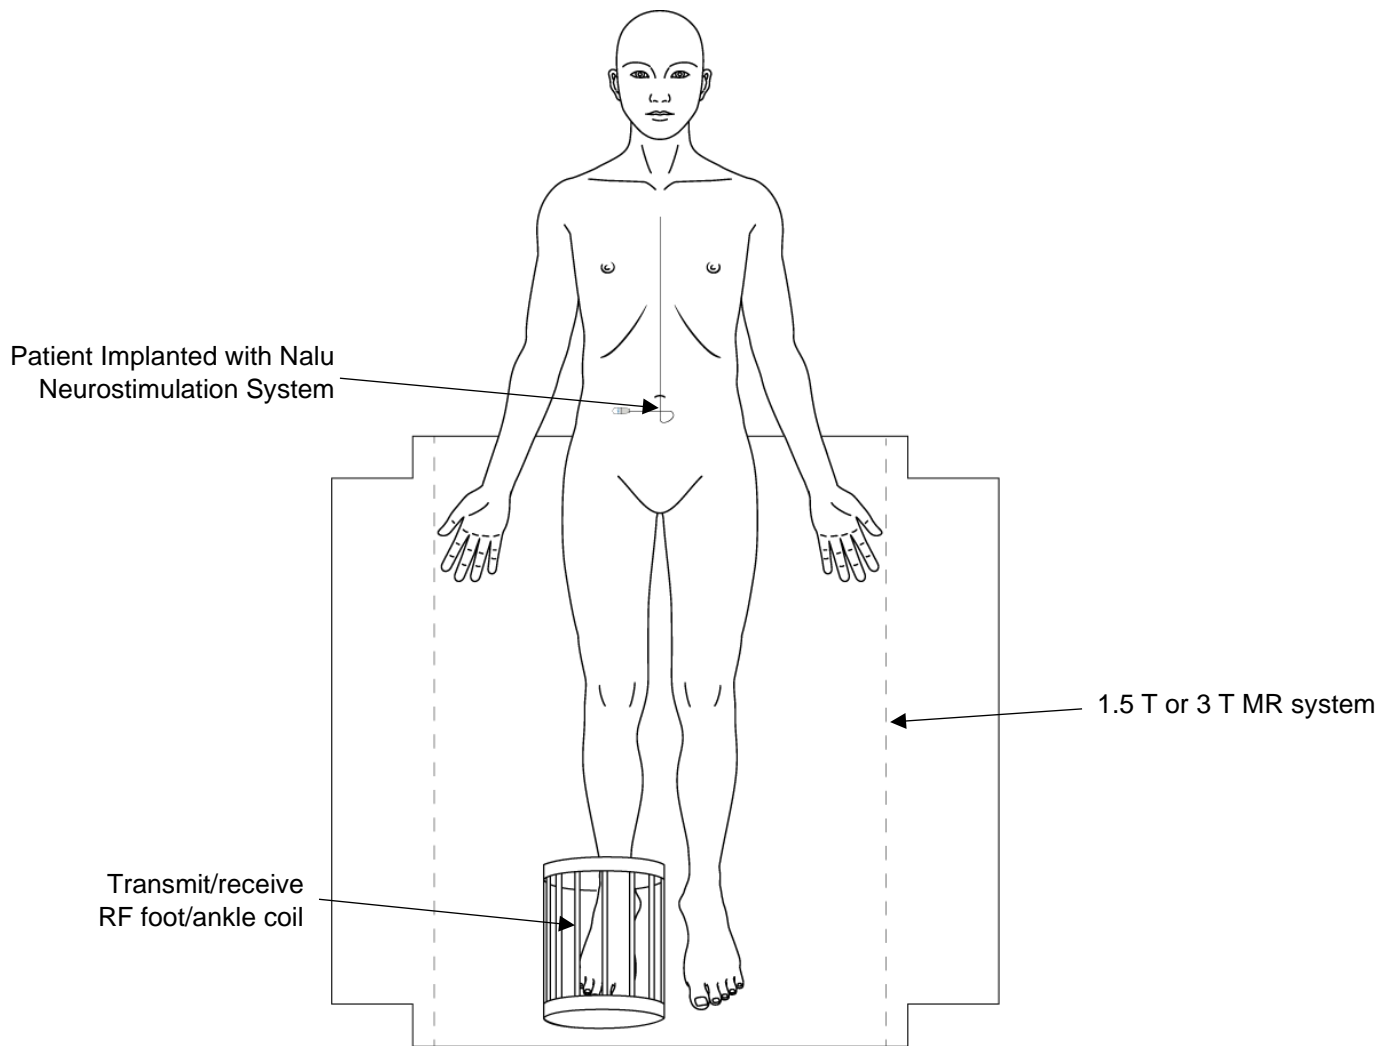

**Figure 2b**



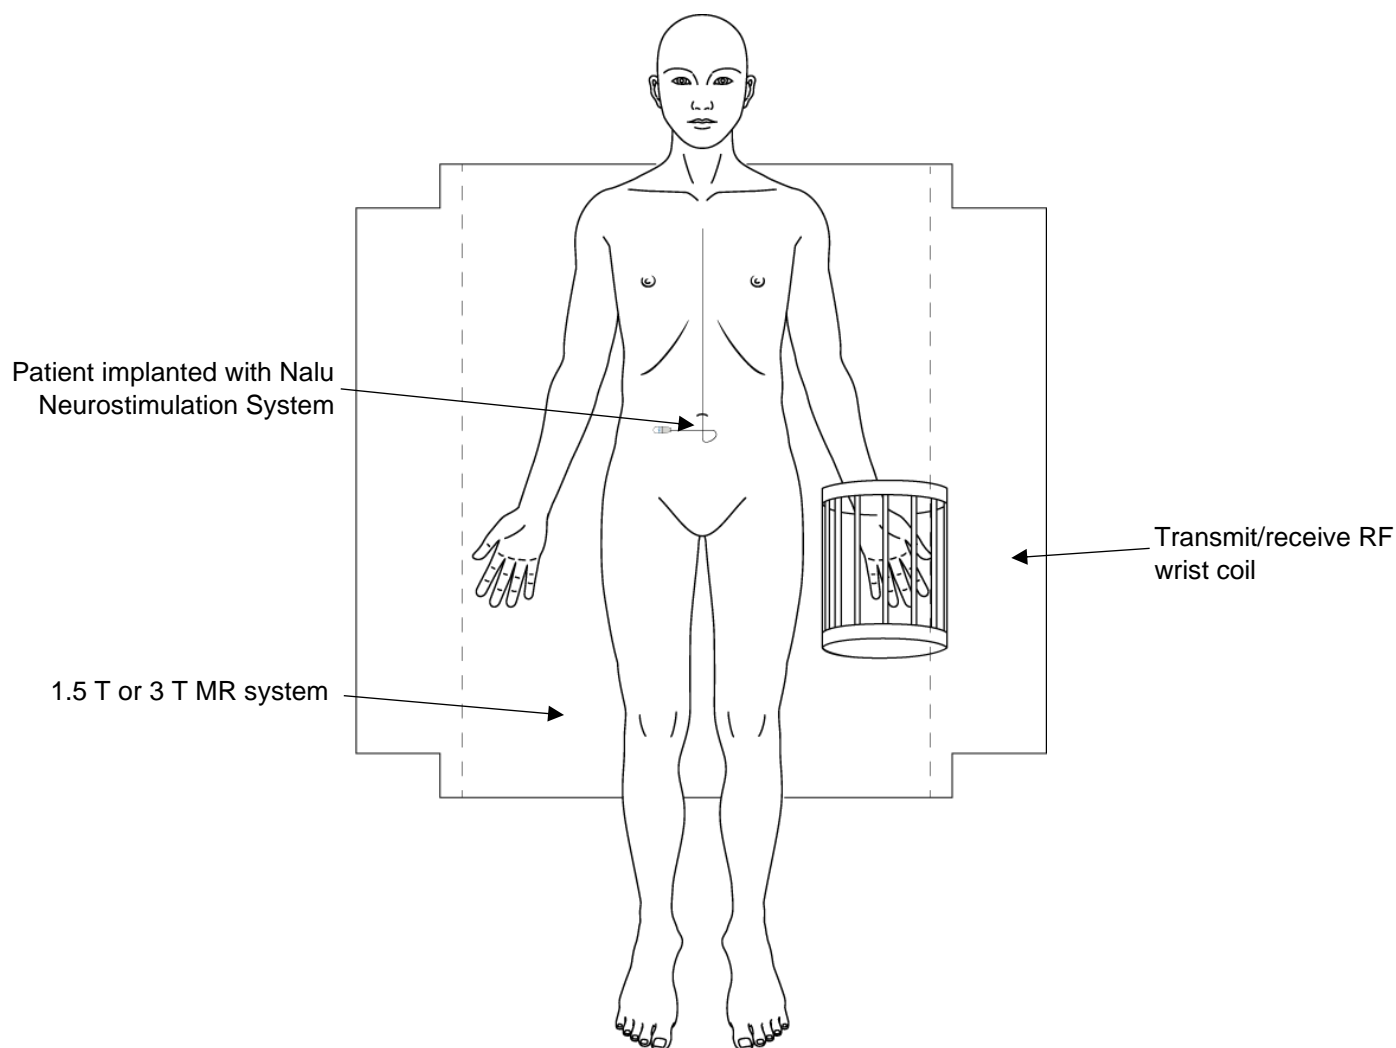


**Figure 2c**

**Figure 2.** Extremity MRI examinations are permitted using a 1.5 T or 3 T MRI system and a transmit/receive RF extremity coil (e.g., knee, foot/ankle, wrist). No part of the implanted Nalu Neurostimulation System may be within the transmit/receive RF extremity coil. All other aforementioned conditions must be carefully followed. **(a)** Represents an MRI of the knee using a transmit/receive RF knee coil. **(b)** Represents an MRI of the foot or ankle using a transmit/receive RF foot/ankle coil. **(c)** Represents an MRI of wrist using a transmit/receive RF wrist coil.

## PNS Head and Extremities scan using a transmit/receive head and extremities


<b>MR Conditional</b>  	
<b>MRI Safety Information</b> For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury.	
Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T or 3.0 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Head and Extremity
Receive Coil Type	Head and Extremity
RF Conditions	First Level Controlled - Partial body SAR of the exposed body part of 10 W/kg and Head SAR of 3.2 W/kg
Scan Duration	Scan for up to 15 minutes.
Scan Regions	For head/brain MRI examinations, only the transmit/receive RF head coil is permitted for use. No parts of the implanted Nalu Neurostimulation System may be within the transmit/receive RF head coil.
	For extremity MRI examinations, only use a transmit/receive RF coil that includes a knee, foot/ankle, or wrist transmit/receive RF coil. <b>No part of the implanted Nalu Neurostimulation System may be within one of these transmit/receive RF coils.</b>
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may result in the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

# WHOLE-BODY MRI LABELING

## How to Determine the Patient's Whole-Body MR Conditionality

This manual walks through a series of questions about the patient's implant to generate a lead code, unique to each implanted lead. If the patient has one implanted lead, one lead code will be generated. If the patient has two implanted leads, two lead codes will be generated. This lead code will then be used to determine what Whole-Body MR conditionality applies to the patient.

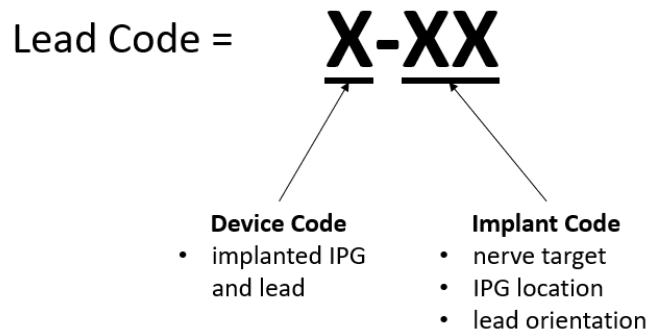

### Step 1 – Select the Device Configuration

Using the Device Configuration table on page 13, find the number that corresponds to the implanted IPG and lead. This number is the patient's device code and the first digit of the patient's lead code.

If the patient has two leads connected to the IPG, repeat Step 1 through 3 for each lead.

If the implanted IPG and lead combination does not appear in the Device Configuration table, then it is MR Unsafe.

*Example 1a:* The patient has a Dual 4 Ported IPG (11007-002) with a 25 cm Tined Lead (12005-025), so the patient's device code is **1-**.

*Example 1b:* The patient has a Single 8 Ported IPG (11003-002) with a 60 cm Multilumen Lead (12001-060), so it is MR Unsafe.

### Step 2 – Select the Nerve Target

After selecting the implanted Device Configuration, go to list of Nerve Targets on page 14, and select the nerve being stimulated by the lead. This will lead to a decision tree applicable to the patient's Nerve Target.

If the nerve being stimulated by the lead is not listed, then it is MR Unsafe.

*Example 2a:* The patient's lead is stimulating the Axillary nerve, so the applicable decision tree is on page 15.

*Example 2b:* The patient's lead is stimulating the Ilioinguinal nerve, which is not present on the Nerve Target list, so it is MR Unsafe.

### Step 3 – Select the IPG Location and Orientation of the Lead's Stimulating Contacts

After selecting the Nerve Target and navigating to the page containing the applicable decision tree, answer the questions in the decision tree to find the patient's implant code. This implant code will be the last two digits of the patient's lead code. The first question asks where the IPG is implanted. If the IPG implant location is not listed or uncertain, select "Other." The second question asks what the orientation of the lead's stimulating contacts is. If the orientation is not clear, select "Uncertain."

*Example 3a:* The patient has a Single 8 Ported IPG (11003-002) with a 40 cm Multilumen Lead (12001-040) stimulating the Sciatic nerve. The IPG is implanted in the lateral thigh, and the stimulating contacts are oriented perpendicular at the popliteal. The lead code for this patient's implant is **6-26**.

*Example 3b:* The patient has a Dual 4 Ported IPG (11007-002) with two 40 cm Tined Leads (12005-025). One lead is stimulating the Axillary nerve and the other is stimulating the Suprascapular nerve. The IPG is implanted on the posterior shoulder over the trapezius. The lead stimulating the Axillary nerve is oriented parallel to the nerve. This lead's code is **2-09**. The lead stimulating the Suprascapular nerve is oriented medial to lateral. This lead's code is **2-46**.

#### Step 4 – Use the Look Up Table

After generating a lead code for all implanted leads, use the corresponding Look Up Table to identify the appropriate label for the patient.

If the patient has one implanted lead, use the Look Up Table starting on page 24. Look through the first column to find the row that matches the lead code that was generated. The second cell of that row lists the appropriate label code for the patient's implant.

If the patient has two implanted leads, use the Look Up Table starting on page 29. Find the column that corresponds to the lead code generated for the first lead. Then find the row that corresponds to the lead code generated for the second lead. The cell that intersects the identified row and column lists the appropriate label code for the patient's implant.

*Example 4a:* The patient has a single implanted lead with lead code **1-05**. Using the Look Up Table starting on page 24, the appropriate label code was identified as **LBL-031**.

*Example 4b:* The patient has two implanted leads with lead codes **2-09** and **2-46**. Using the Look Up Table starting on page 29, the appropriate label code was identified as **LBL-015**.













#### Step 5 – Go to the Identified Label

After navigating the Look Up Table and identifying the appropriate label code for the patient's implant, use the list of Labels starting on page 46 to find the page corresponding to that label code. This page will display the Whole-Body MR Conditionality for the patient's implant.

*Example 5:* The appropriate label code for the patient's implant was identified to be **LBL-034**. The Whole-Body MR Conditionality for this patient can be found on page 82.

**For patients with more than one implanted Nalu Neurostimulation System:** Repeat Steps 1-5 for each implanted Nalu Neurostimulation System. The MRI examination must adhere to the conditions specified in all applicable labels. The most restrictive SAR value should be used for each specified Zone.


## Device Configurations


Device Code	Implanted IPG and Lead
1	Dual 4 Ported IPG (11007-002) + 25 cm Tined Lead (12005-025) 
2	Dual 4 Ported IPG (11007-002) + 40 cm Tined Lead (12005-040) 
3	Dual 8 Ported IPG (11004-002) + 40 cm Multilumen Lead (12001-040) 
	Dual 8 Integrated IPG, 40 cm (11002-040) 
	Dual 8 Alternate Pitch IPG (11009-002) + 40 cm Alternate Pitch Lead (12010-040) 
4	Single 4 Ported IPG (11006-002) + 25 cm Tined Lead (12005-025) 
	Single 4 Integrated IPG, 25 cm Tined (11005-025) 
5	Single 4 Ported IPG (11006-002) + 40 cm Tined Lead (12005-040) 
	Single 4 Integrated IPG, 40 cm Tined (11005-040) 
6	Single 8 Ported IPG (11003-002) + 40 cm Multilumen Lead (12001-040) 
	Single 8 Integrated IPG, 40 cm (11001-040) 
	Any device configuration not listed above is MRI Unsafe.

## **Nerve Target**

AXILLARY.....	PAGE 15
GENICULAR.....	PAGE 16
SAPHENOUS .....	PAGE 17
SCIATIC.....	PAGE 18
SUPERIOR CLUNEAL.....	PAGE 19
SUPRASCAPULAR .....	PAGE 20
TIBIAL.....	PAGE 21
SCS (SPINAL CORD STIMULATION) .....	PAGE 22
SACRAL .....	PAGE 23


Axillary

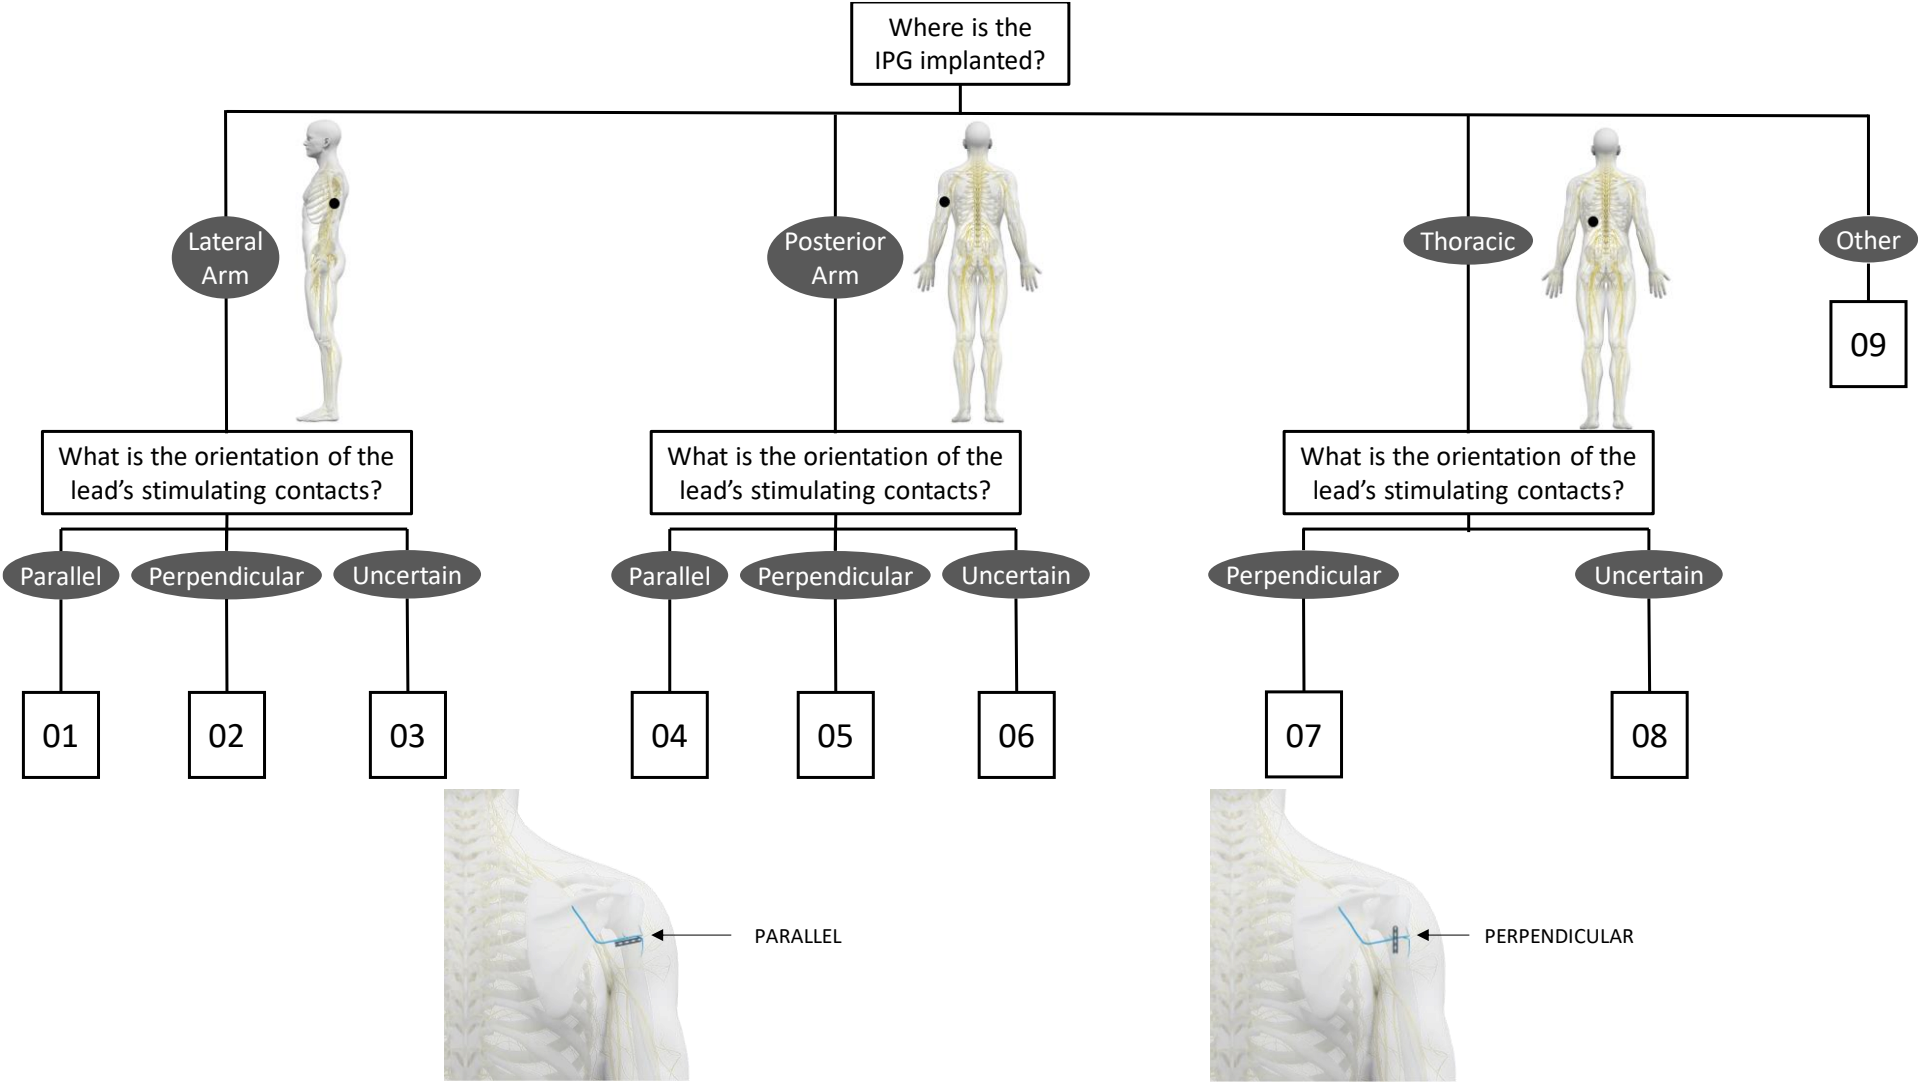


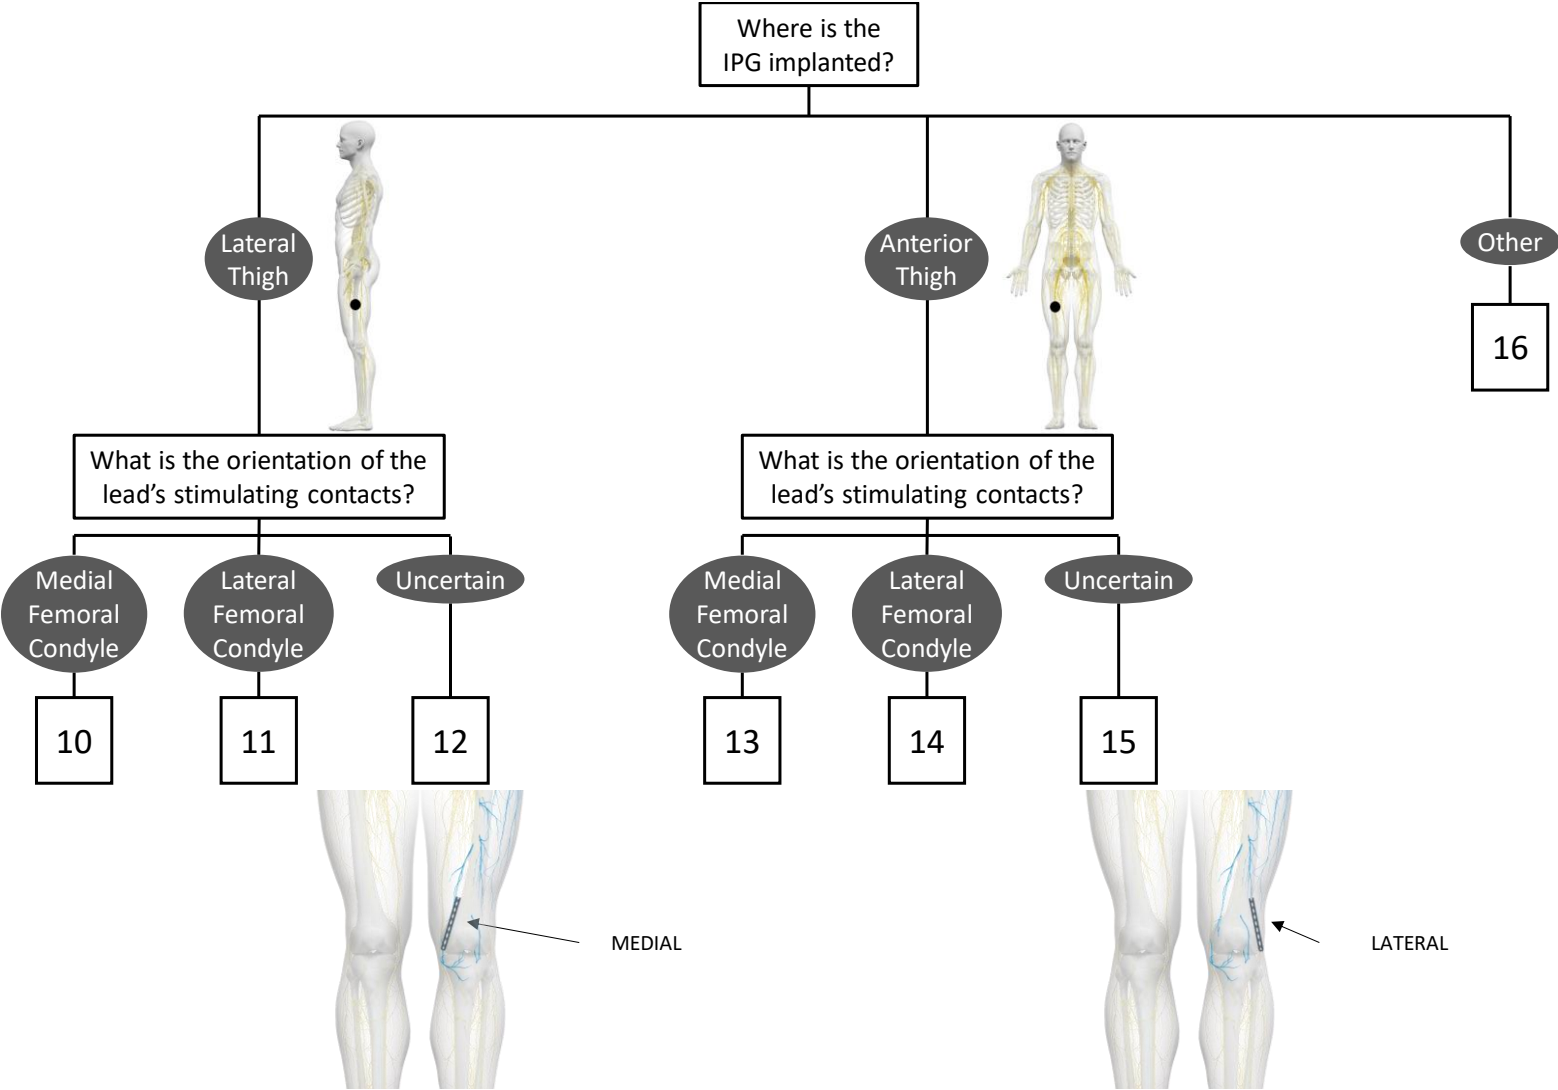




Saphenous

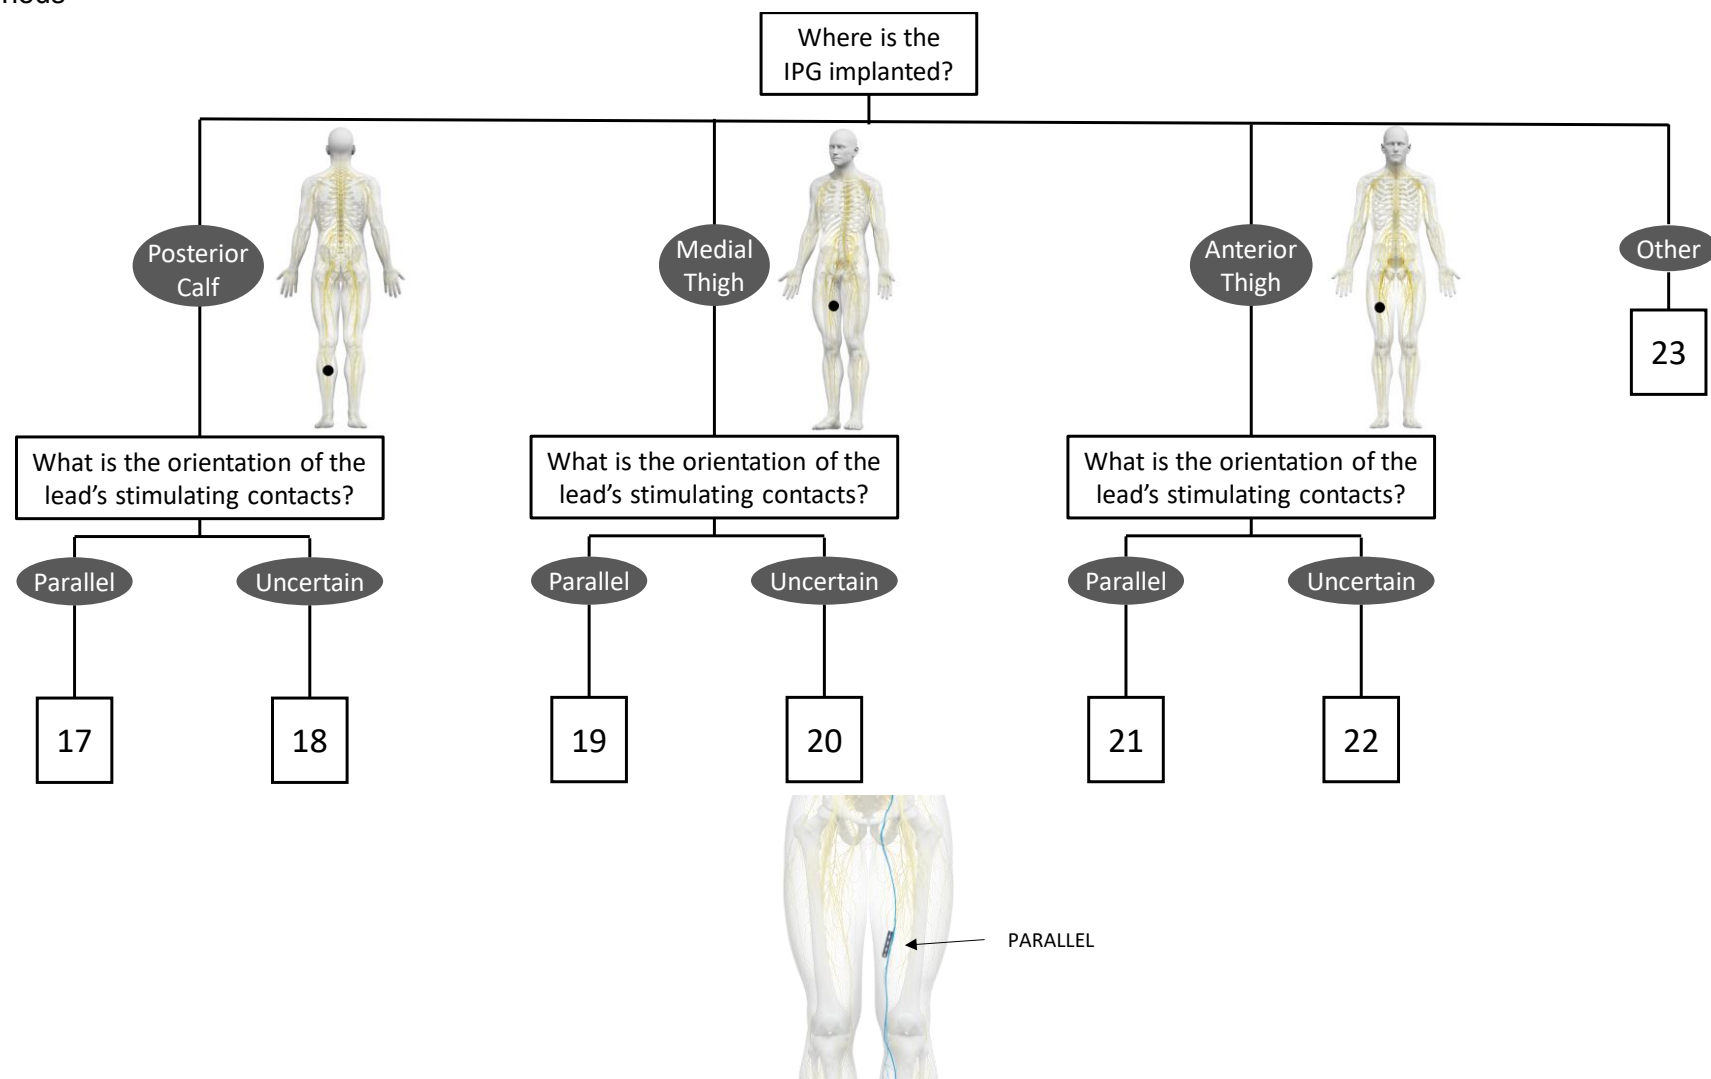


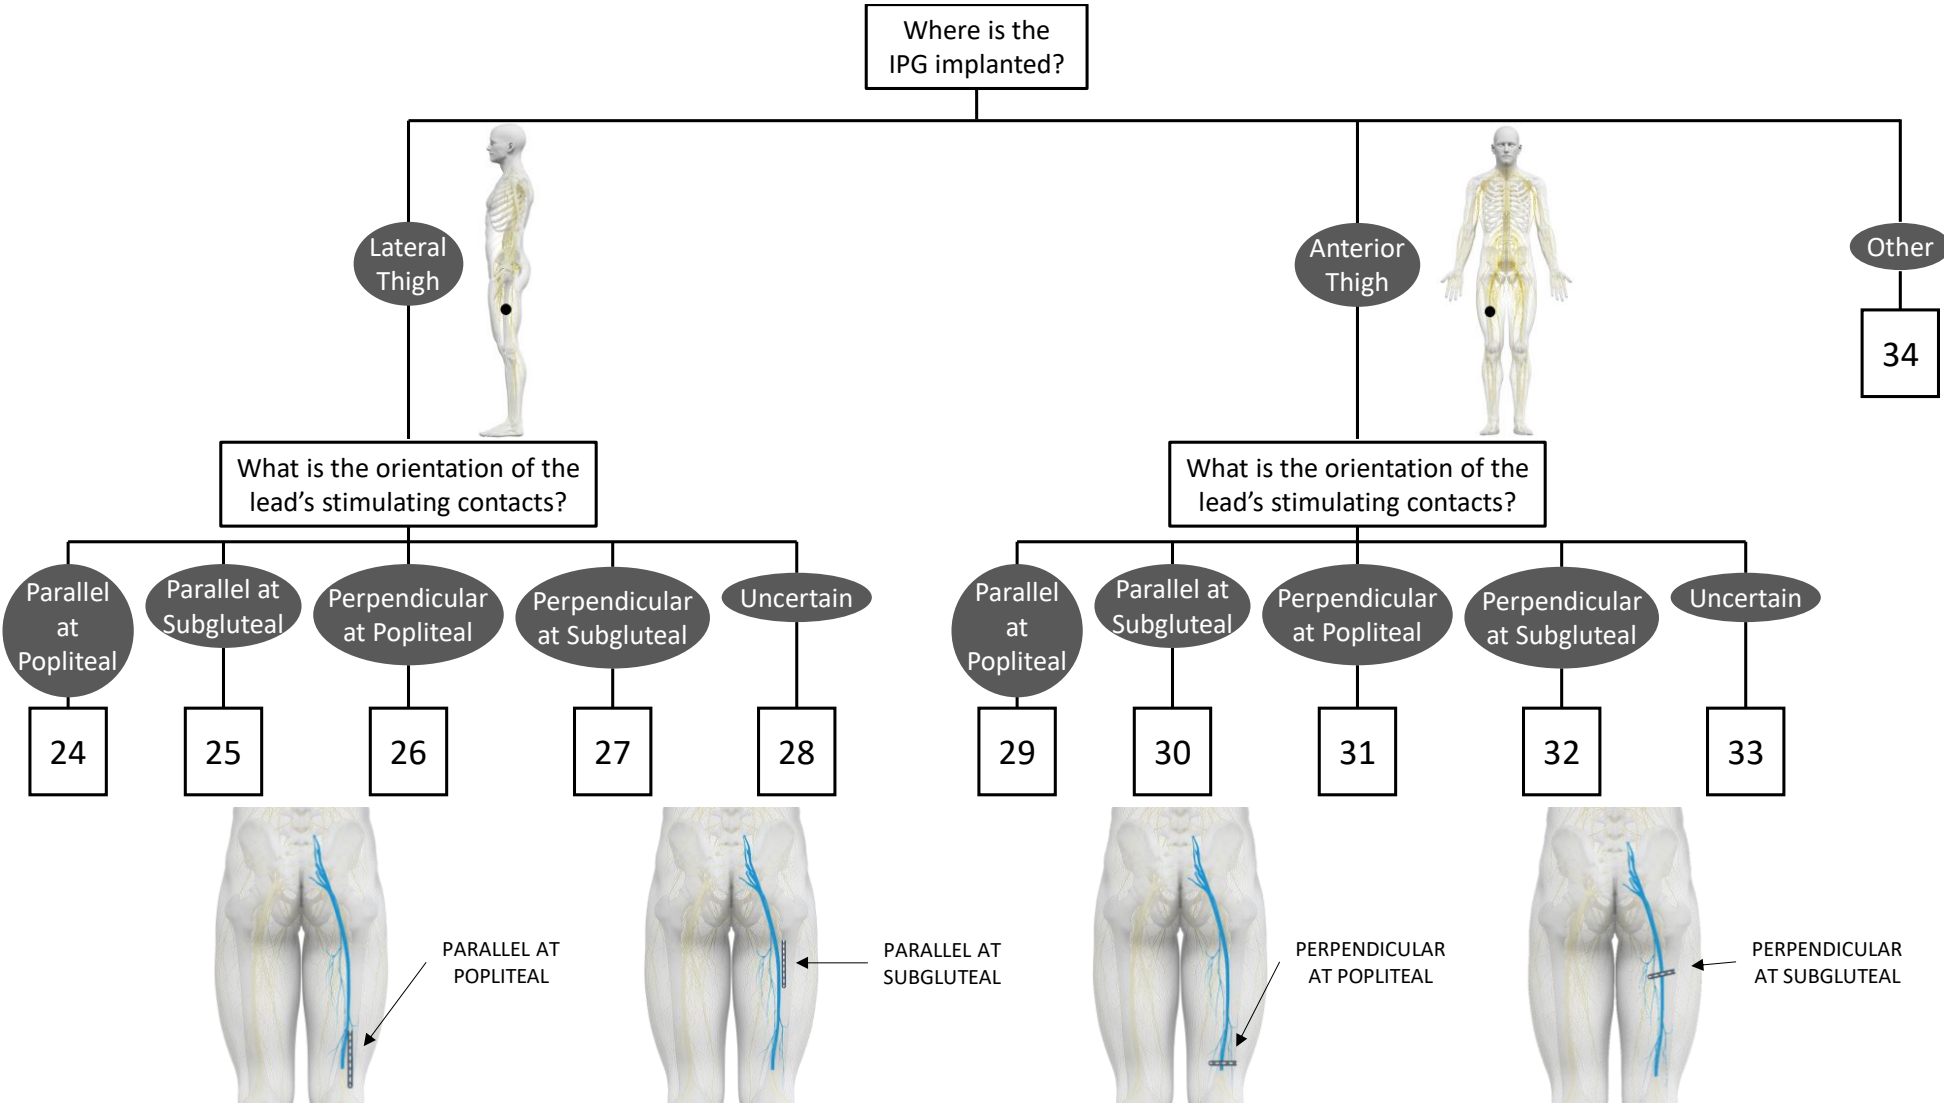


Superior Cluneal

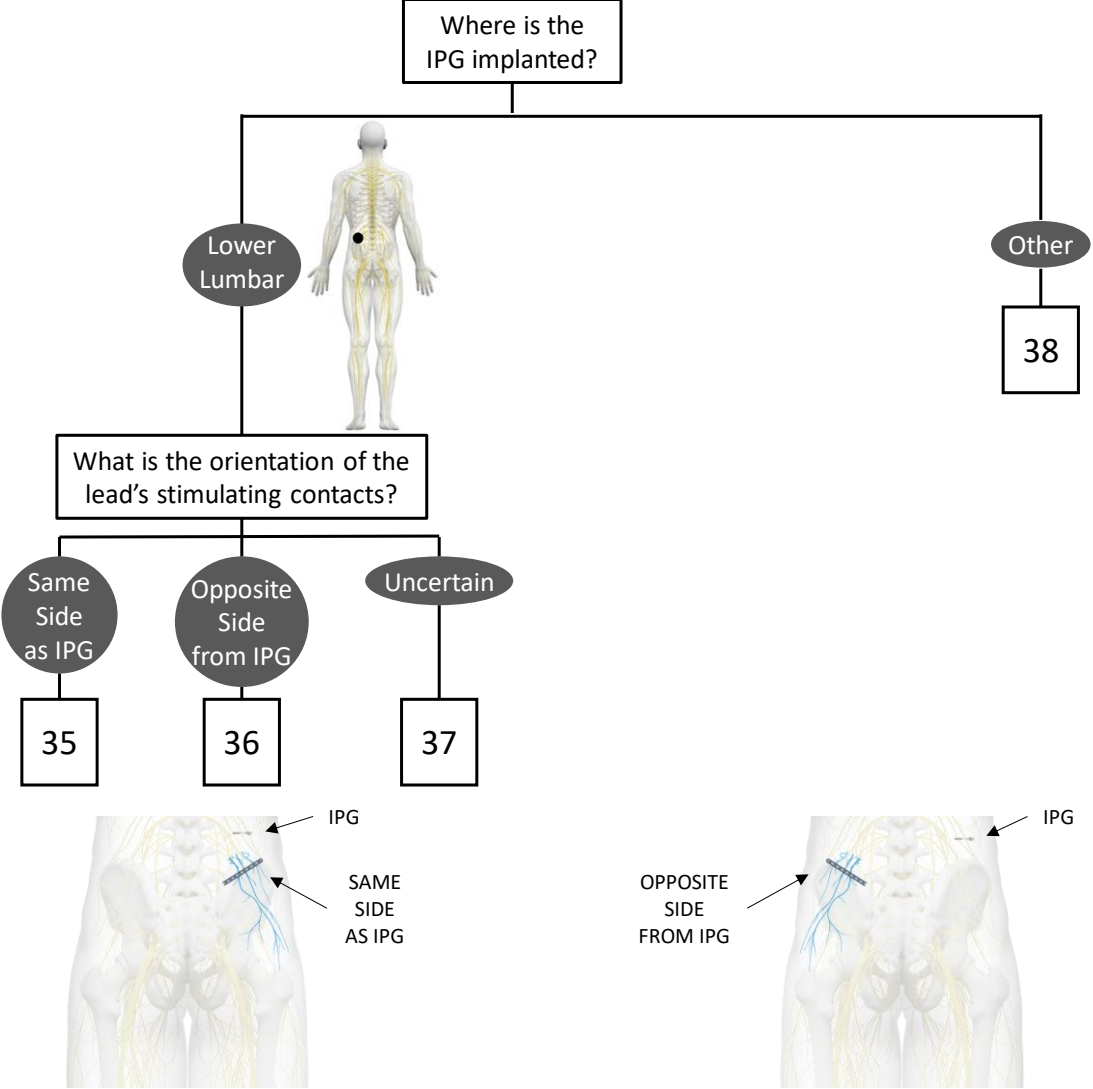



Suprascapular

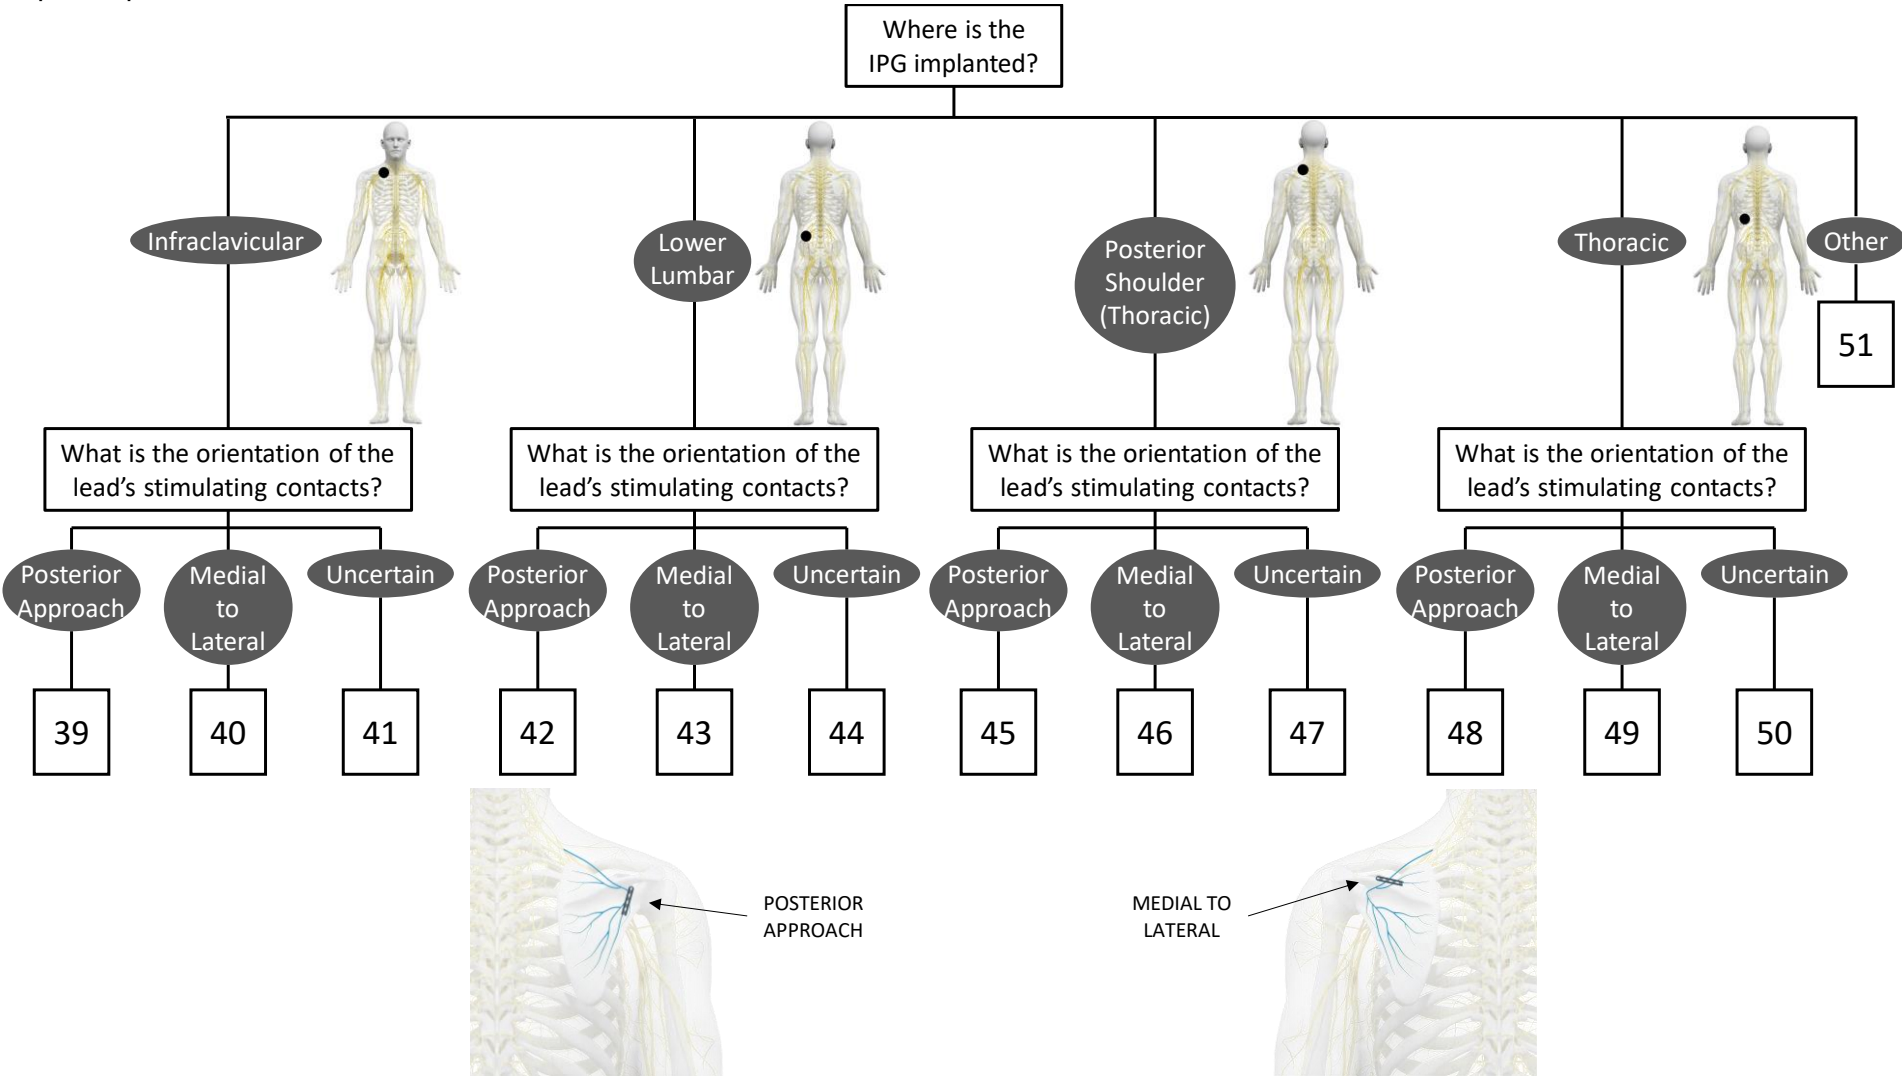

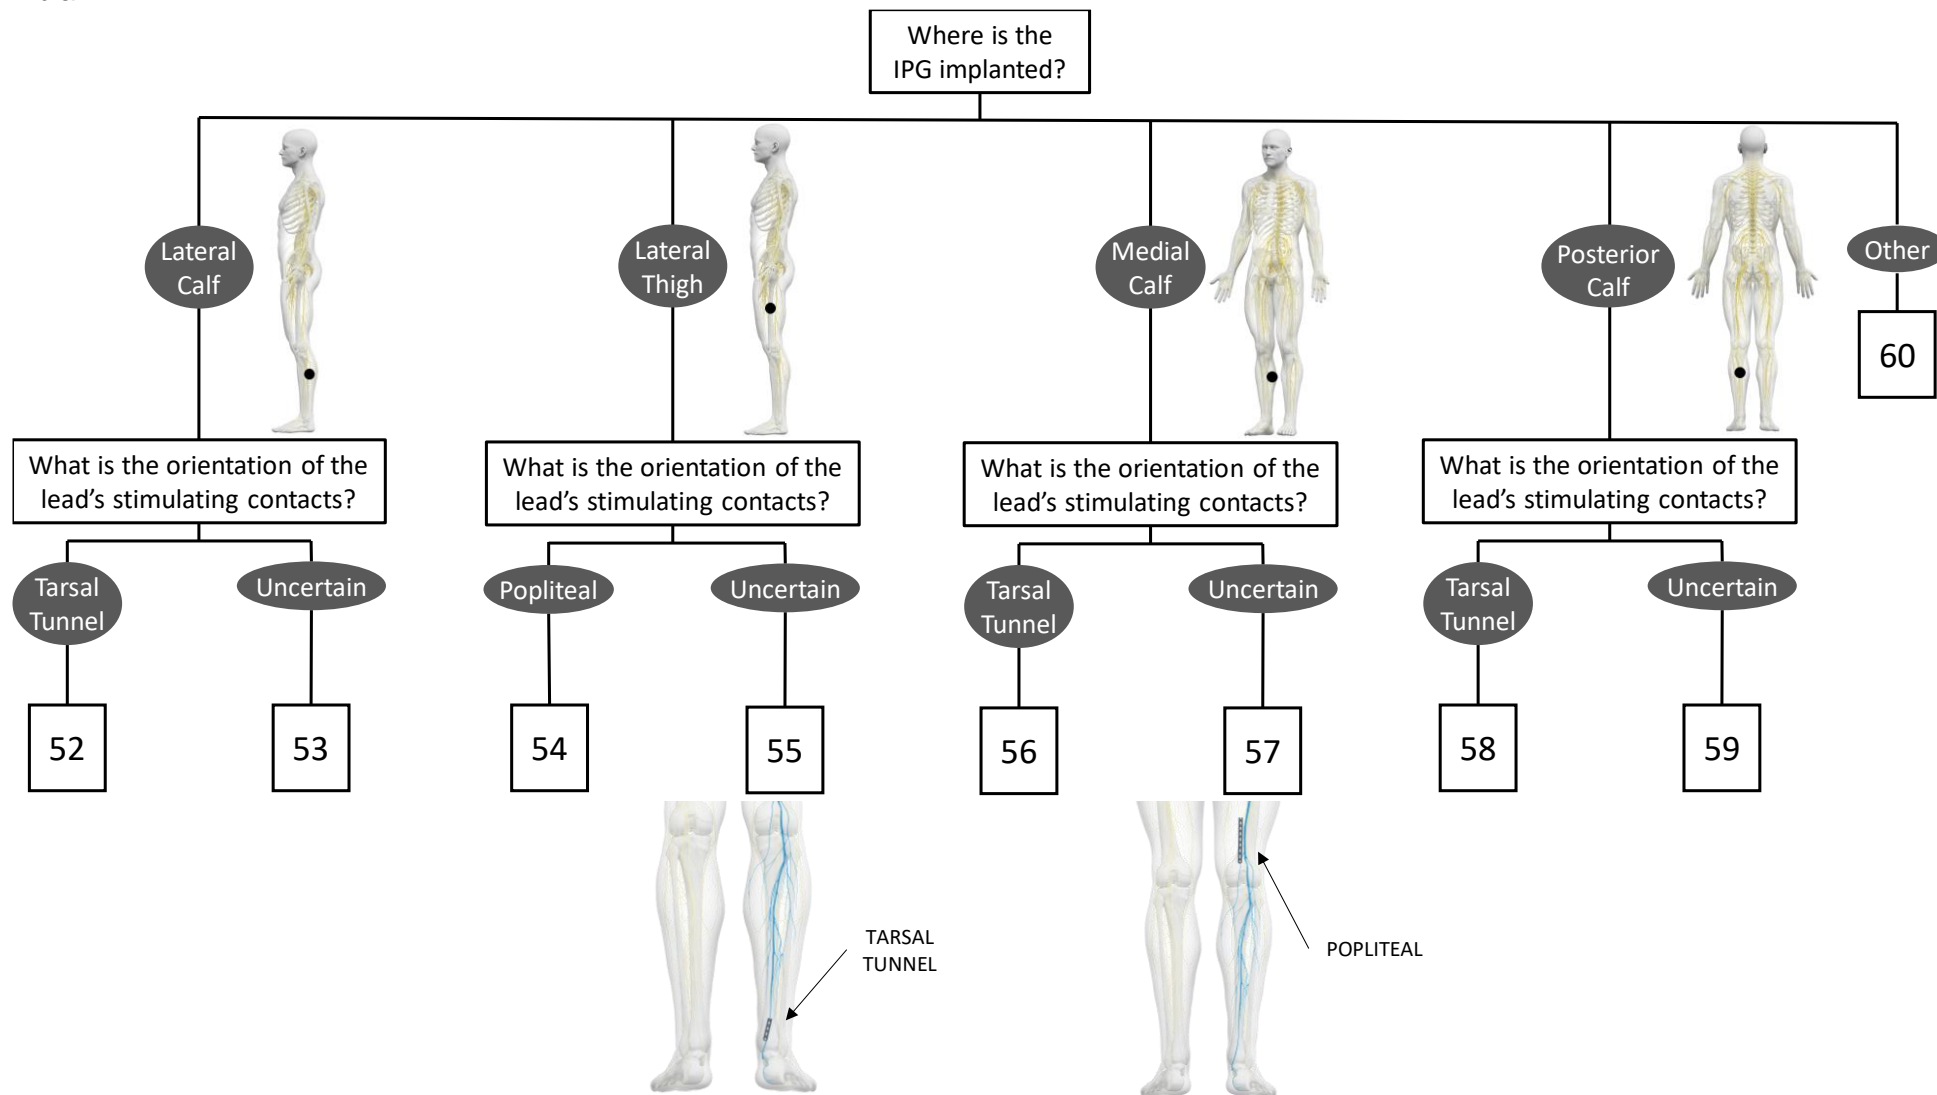

SCS (Spinal Cord Stimulation)

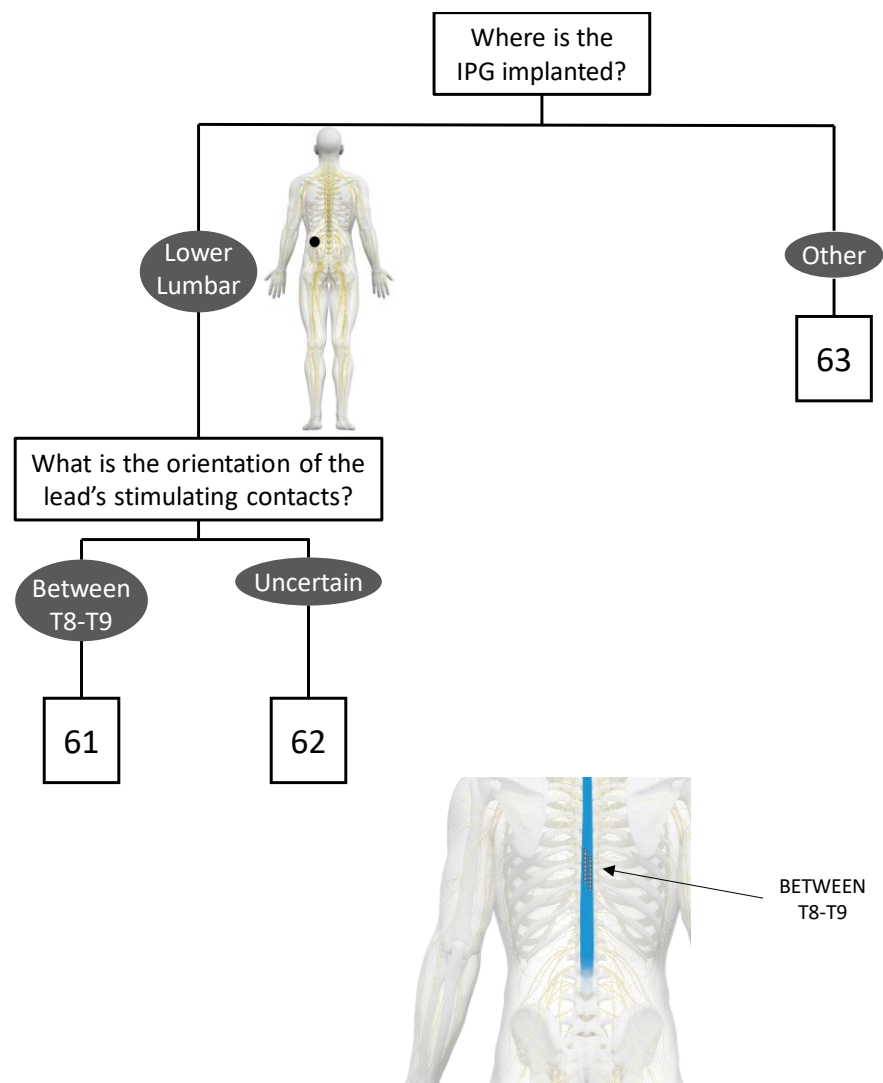

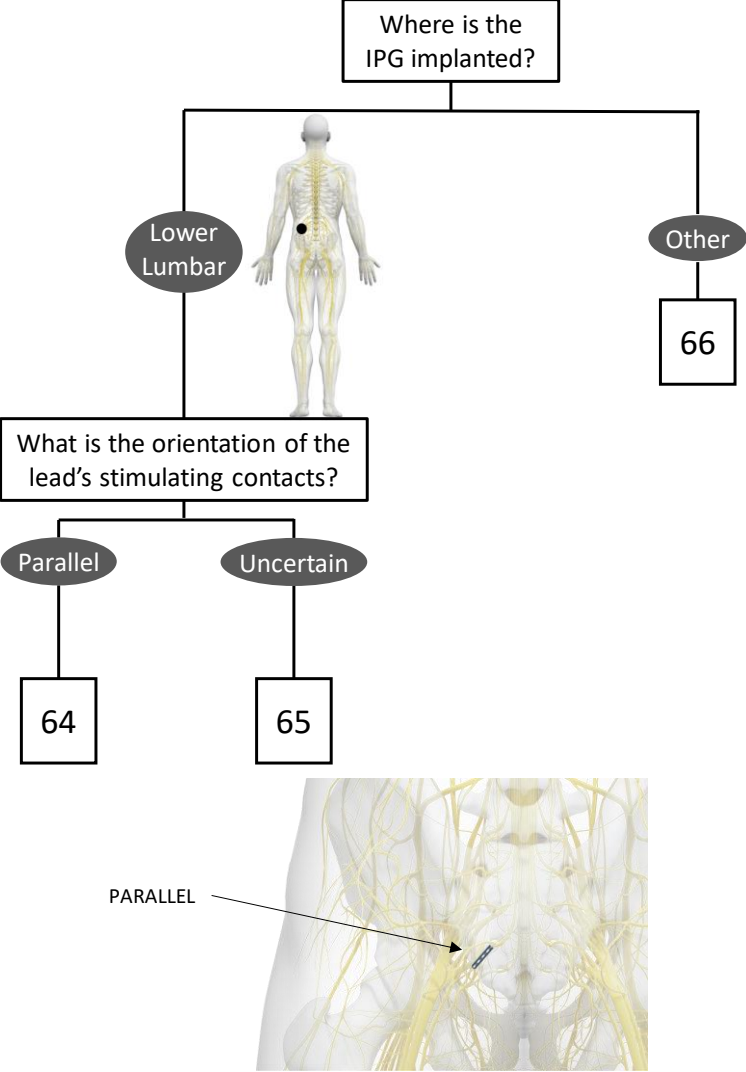

## Single Lead Look-Up Table

Lead Code	Label Code
1-01	LBL-047
1-02	LBL-051
1-03	LBL-047
1-04	LBL-040
1-05	LBL-031
1-06	LBL-031
1-07	LBL-031
1-08	LBL-031
1-09	LBL-031
1-10	LBL-060
1-11	LBL-002
1-12	LBL-002
1-13	LBL-002
1-14	LBL-002
1-15	LBL-002
1-16	LBL-002
1-17	LBL-001
1-18	LBL-001
1-19	LBL-082
1-20	LBL-082
1-21	LBL-067
1-22	LBL-067
1-23	LBL-067
1-24	LBL-060
1-25	LBL-081
1-26	LBL-058
1-27	LBL-088
1-28	LBL-058
1-29	LBL-073
1-30	LBL-098
1-31	LBL-071
1-32	LBL-099
1-33	LBL-071
1-34	LBL-058
1-35	LBL-001
1-36	LBL-001
1-37	LBL-001
1-38	LBL-001
1-39	LBL-023
1-40	LBL-023
1-41	LBL-023

Lead Code	Label Code
1-42	LBL-020
1-43	LBL-020
1-44	LBL-020
1-45	LBL-025
1-46	LBL-024
1-47	LBL-024
1-48	LBL-020
1-49	LBL-020
1-50	LBL-020
1-51	LBL-020
1-52	LBL-002
1-53	LBL-002
1-54	LBL-002
1-55	LBL-002
1-56	LBL-060
1-57	LBL-060
1-58	LBL-053
1-59	LBL-053
1-60	LBL-002
1-61	LBL-004
1-62	LBL-004
1-63	LBL-004
1-64	LBL-005
1-65	LBL-005
1-66	LBL-005
2-01	LBL-001
2-02	LBL-042
2-03	LBL-042
2-04	LBL-050
2-05	LBL-027
2-06	LBL-027
2-07	LBL-030
2-08	LBL-030
2-09	LBL-027
2-10	LBL-076
2-11	LBL-061
2-12	LBL-061
2-13	LBL-063
2-14	LBL-002
2-15	LBL-002
2-16	LBL-002



Lead Code	Label Code
2-17	LBL-075
2-18	LBL-075
2-19	LBL-094
2-20	LBL-094
2-21	LBL-077
2-22	LBL-077
2-23	LBL-075
2-24	LBL-106
2-25	LBL-112
2-26	LBL-054
2-27	LBL-001
2-28	LBL-054
2-29	LBL-072
2-30	LBL-097
2-31	LBL-070
2-32	LBL-111
2-33	LBL-070
2-34	LBL-054
2-35	LBL-001
2-36	LBL-113
2-37	LBL-113
2-38	LBL-113
2-39	LBL-010
2-40	LBL-003
2-41	LBL-003
2-42	LBL-003
2-43	LBL-003
2-44	LBL-003
2-45	LBL-018
2-46	LBL-015
2-47	LBL-015
2-48	LBL-037
2-49	LBL-017
2-50	LBL-017
2-51	LBL-003
2-52	LBL-067
2-53	LBL-067
2-54	LBL-057
2-55	LBL-057
2-56	LBL-062
2-57	LBL-062
2-58	LBL-069

Lead Code	Label Code
2-59	LBL-069
2-60	LBL-057
2-61	LBL-004
2-62	LBL-004
2-63	LBL-004
2-64	LBL-005
2-65	LBL-005
2-66	LBL-005
3-01	LBL-001
3-02	LBL-048
3-03	LBL-048
3-04	LBL-001
3-05	LBL-045
3-06	LBL-045
3-07	LBL-041
3-08	LBL-041
3-09	LBL-041
3-10	LBL-086
3-11	LBL-053
3-12	LBL-053
3-13	LBL-065
3-14	LBL-002
3-15	LBL-002
3-16	LBL-002
3-17	LBL-102
3-18	LBL-102
3-19	LBL-110
3-20	LBL-110
3-21	LBL-095
3-22	LBL-095
3-23	LBL-095
3-24	LBL-096
3-25	LBL-001
3-26	LBL-078
3-27	LBL-001
3-28	LBL-078
3-29	LBL-070
3-30	LBL-101
3-31	LBL-092
3-32	LBL-001
3-33	LBL-070
3-34	LBL-070

Lead Code	Label Code
3-35	LBL-001
3-36	LBL-115
3-37	LBL-115
3-38	LBL-115
3-39	LBL-013
3-40	LBL-011
3-41	LBL-011
3-42	LBL-017
3-43	LBL-003
3-44	LBL-003
3-45	LBL-028
3-46	LBL-022
3-47	LBL-022
3-48	LBL-035
3-49	LBL-021
3-50	LBL-021
3-51	LBL-003
3-52	LBL-063
3-53	LBL-063
3-54	LBL-053
3-55	LBL-053
3-56	LBL-061
3-57	LBL-061
3-58	LBL-068
3-59	LBL-068
3-60	LBL-053
3-61	LBL-116
3-62	LBL-004
3-63	LBL-004
3-64	LBL-005
3-65	LBL-005
3-66	LBL-005
4-01	LBL-044
4-02	LBL-001
4-03	LBL-044
4-04	LBL-032
4-05	LBL-001
4-06	LBL-032
4-07	LBL-032
4-08	LBL-032
4-09	LBL-032
4-10	LBL-002

Lead Code	Label Code
4-11	LBL-002
4-12	LBL-002
4-13	LBL-002
4-14	LBL-002
4-15	LBL-002
4-16	LBL-002
4-17	LBL-001
4-18	LBL-001
4-19	LBL-074
4-20	LBL-074
4-21	LBL-059
4-22	LBL-059
4-23	LBL-059
4-24	LBL-002
4-25	LBL-076
4-26	LBL-059
4-27	LBL-085
4-28	LBL-002
4-29	LBL-066
4-30	LBL-091
4-31	LBL-079
4-32	LBL-088
4-33	LBL-066
4-34	LBL-002
4-35	LBL-001
4-36	LBL-001
4-37	LBL-001
4-38	LBL-001
4-39	LBL-033
4-40	LBL-033
4-41	LBL-033
4-42	LBL-012
4-43	LBL-012
4-44	LBL-012
4-45	LBL-001
4-46	LBL-014
4-47	LBL-014
4-48	LBL-012
4-49	LBL-012
4-50	LBL-012
4-51	LBL-012
4-52	LBL-002

Lead Code	Label Code
4-53	LBL-002
4-54	LBL-002
4-55	LBL-002
4-56	LBL-052
4-57	LBL-052
4-58	LBL-002
4-59	LBL-002
4-60	LBL-002
4-61	LBL-004
4-62	LBL-004
4-63	LBL-004
4-64	LBL-117
4-65	LBL-005
4-66	LBL-005
5-01	LBL-001
5-02	LBL-046
5-03	LBL-046
5-04	LBL-001
5-05	LBL-026
5-06	LBL-026
5-07	LBL-039
5-08	LBL-039
5-09	LBL-026
5-10	LBL-062
5-11	LBL-063
5-12	LBL-062
5-13	LBL-052
5-14	LBL-054
5-15	LBL-052
5-16	LBL-052
5-17	LBL-083
5-18	LBL-083
5-19	LBL-081
5-20	LBL-081
5-21	LBL-072
5-22	LBL-072
5-23	LBL-072
5-24	LBL-089
5-25	LBL-104
5-26	LBL-056
5-27	LBL-105
5-28	LBL-056

Lead Code	Label Code
5-29	LBL-079
5-30	LBL-090
5-31	LBL-077
5-32	LBL-103
5-33	LBL-077
5-34	LBL-056
5-35	LBL-001
5-36	LBL-114
5-37	LBL-114
5-38	LBL-114
5-39	LBL-019
5-40	LBL-010
5-41	LBL-010
5-42	LBL-003
5-43	LBL-003
5-44	LBL-003
5-45	LBL-017
5-46	LBL-034
5-47	LBL-017
5-48	LBL-029
5-49	LBL-016
5-50	LBL-016
5-51	LBL-003
5-52	LBL-055
5-53	LBL-055
5-54	LBL-058
5-55	LBL-058
5-56	LBL-084
5-57	LBL-084
5-58	LBL-064
5-59	LBL-064
5-60	LBL-055
5-61	LBL-004
5-62	LBL-004
5-63	LBL-004
5-64	LBL-001
5-65	LBL-005
5-66	LBL-005
6-01	LBL-001
6-02	LBL-001
6-03	LBL-001
6-04	LBL-001

Lead Code	Label Code
6-05	LBL-001
6-06	LBL-001
6-07	LBL-049
6-08	LBL-049
6-09	LBL-049
6-10	LBL-063
6-11	LBL-002
6-12	LBL-002
6-13	LBL-053
6-14	LBL-002
6-15	LBL-002
6-16	LBL-002
6-17	LBL-001
6-18	LBL-001
6-19	LBL-108
6-20	LBL-108
6-21	LBL-107
6-22	LBL-107
6-23	LBL-107
6-24	LBL-093
6-25	LBL-001
6-26	LBL-100
6-27	LBL-001
6-28	LBL-093
6-29	LBL-080
6-30	LBL-109
6-31	LBL-001
6-32	LBL-001
6-33	LBL-080
6-34	LBL-080
6-35	LBL-001

Lead Code	Label Code
6-36	LBL-001
6-37	LBL-001
6-38	LBL-001
6-39	LBL-043
6-40	LBL-031
6-41	LBL-031
6-42	LBL-003
6-43	LBL-003
6-44	LBL-003
6-45	LBL-001
6-46	LBL-034
6-47	LBL-034
6-48	LBL-038
6-49	LBL-036
6-50	LBL-036
6-51	LBL-003
6-52	LBL-054
6-53	LBL-054
6-54	LBL-002
6-55	LBL-002
6-56	LBL-087
6-57	LBL-087
6-58	LBL-060
6-59	LBL-060
6-60	LBL-002
6-61	LBL-004
6-62	LBL-004
6-63	LBL-004
6-64	LBL-005
6-65	LBL-005
6-66	LBL-005

## Dual Lead Look-Up Table

1-01 TO 1-33, 1-01 TO 1-33 .....	PAGE 30
1-01 TO 1-33, 1-34 TO 1-66 .....	PAGE 31
1-34 TO 1-66, 1-01 TO 1-33 .....	PAGE 32
1-34 TO 1-66, 1-34 TO 1-66 .....	PAGE 33
1-01 TO 1-33, 2-01 TO 2-33 .....	PAGE 34
1-01 TO 1-33, 2-34 TO 2-66 .....	PAGE 35
1-34 TO 1-66, 2-01 TO 2-33 .....	PAGE 36
1-34 TO 1-66, 2-34 TO 2-36 .....	PAGE 37
2-01 TO 2-33, 2-01 TO 2-33 .....	PAGE 38
2-01 TO 2-33, 2-34 TO 2-66 .....	PAGE 39
2-34 TO 2-66, 2-01 TO 2-33 .....	PAGE 40
2-34 TO 2-66, 2-34 TO 2-66 .....	PAGE 41
3-01 TO 3-33, 3-01 TO 3-33 .....	PAGE 42
3-01 TO 3-33, 3-34 TO 3-66 .....	PAGE 43
3-34 TO 3-66, 3-01 TO 3-33 .....	PAGE 44
3-34 TO 3-66, 3-34 TO 3-66 .....	PAGE 45

1-01 to 1-33, 1-01 to 1-33

	1-01	1-02	1-03	1-04	1-05	1-06	1-07	1-08	1-09	1-10	1-11	1-12	1-13	1-14	1-15	1-16	1-17	1-18	1-19	1-20	1-21	1-22	1-23	1-24	1-25	1-26	1-27	1-28	1-29	1-30	1-31	1-32	1-33
1-01	LBL-047	LBL-047	LBL-047	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-02	LBL-047	LBL-051	LBL-047	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-03	LBL-047	LBL-047	LBL-047	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-04	MR	MR	MR	LBL-040	LBL-031	LBL-031	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-05	MR	MR	MR	LBL-031	LBL-031	LBL-031	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-06	MR	MR	MR	LBL-031	LBL-031	LBL-031	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-07	MR	MR	MR	MR	MR	MR	LBL-031	LBL-031	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-08	MR	MR	MR	MR	MR	MR	LBL-031	LBL-031	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-09	MR	MR	MR	MR	MR	MR	MR	MR	LBL-031	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-10	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-060	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-060	LBL-060	LBL-060	LBL-058	LBL-060	LBL-058	MR	MR	MR	MR
1-11	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR
1-12	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR
1-13	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	
1-14	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	
1-15	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	
1-16	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-17	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-001	LBL-001	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-18	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-001	LBL-001	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-19	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	LBL-082	LBL-082	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-20	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	LBL-082	LBL-082	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-21	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-22	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-23	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-060	LBL-002	LBL-002	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-24	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-060	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-25	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-060	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-26	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-058	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-27	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-060	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-28	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-058	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-29	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-30	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-31	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-32	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-33	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR

1-01 to 1-33, 1-34 to 1-66

	1-34	1-35	1-36	1-37	1-38	1-39	1-40	1-41	1-42	1-43	1-44	1-45	1-46	1-47	1-48	1-49	1-50	1-51	1-52	1-53	1-54	1-55	1-56	1-57	1-58	1-59	1-60	1-61	1-62	1-63	1-64	1-65	1-66
1-01	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-02	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-03	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-04	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-05	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-06	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-07	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-020	LBL-020	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-08	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-020	LBL-020	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-09	MR	MR	MR	MR	MR	LBL-023	LBL-023	LBL-023	LBL-020	LBL-020	LBL-025	LBL-024	LBL-024	MR	MR	MR	MR	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-10	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-11	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-12	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-13	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR
1-14	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR
1-15	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR
1-16	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	LBL-002	LBL-002	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR
1-17	LBL-058	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR
1-18	LBL-058	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR
1-19	LBL-058	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR
1-20	LBL-058	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR
1-21	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR
1-22	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR
1-23	LBL-058	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	LBL-002	LBL-060	LBL-060	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR
1-24	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-25	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-26	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-27	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-28	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-29	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR
1-30	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR
1-31	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR
1-32	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR
1-33	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR

1-34 to 1-66, 1-01 to 1-33

	1-01	1-02	1-03	1-04	1-05	1-06	1-07	1-08	1-09	1-10	1-11	1-12	1-13	1-14	1-15	1-16	1-17	1-18	1-19	1-20	1-21	1-22	1-23	1-24	1-25	1-26	1-27	1-28	1-29	1-30	1-31	1-32	1-33
1-34	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-058	LBL-058	LBL-058	LBL-058	MR	MR	MR	LBL-058	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-35	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-36	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-37	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-38	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-39	MR	MR	MR	MR	MR	MR	MR	MR	LBL-023	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-40	MR	MR	MR	MR	MR	MR	MR	MR	LBL-023	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-41	MR	MR	MR	MR	MR	MR	MR	MR	LBL-023	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-42	MR	MR	MR	MR	MR	MR	MR	MR	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-43	MR	MR	MR	MR	MR	MR	MR	MR	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-44	MR	MR	MR	MR	MR	MR	MR	MR	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-45	MR	MR	MR	MR	MR	MR	MR	MR	LBL-025	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-46	MR	MR	MR	MR	MR	MR	MR	MR	LBL-024	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-47	MR	MR	MR	MR	MR	MR	MR	MR	LBL-024	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-48	MR	MR	MR	MR	MR	MR	LBL-020	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-49	MR	MR	MR	MR	MR	MR	LBL-020	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-50	MR	MR	MR	MR	MR	MR	LBL-020	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-51	LBL-020	LBL-020	LBL-020	LBL-020	LBL-020	LBL-020	MR	MR	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-52	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-53	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-54	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR
1-55	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR
1-56	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR	MR	LBL-060	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-57	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR	MR	LBL-060	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-58	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-59	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-60	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	LBL-002	MR	MR	LBL-002	LBL-002	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-61	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-62	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-63	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-64	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-65	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-66	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR



1-34 to 1-66, 1-34 to 1-66

	1-34	1-35	1-36	1-37	1-38	1-39	1-40	1-41	1-42	1-43	1-44	1-45	1-46	1-47	1-48	1-49	1-50	1-51	1-52	1-53	1-54	1-55	1-56	1-57	1-58	1-59	1-60	1-61	1-62	1-63	1-64	1-65	1-66
1-34	LBL-058	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	LBL-058	LBL-058	LBL-053	LBL-053	LBL-002	MR	MR	MR	MR	MR	MR
1-35	MR	LBL-001	LBL-001	LBL-001	MR	MR	MR	MR	LBL-020	LBL-020	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-004	LBL-004	MR	LBL-005	LBL-005	MR
1-36	MR	LBL-001	LBL-001	LBL-001	MR	MR	MR	MR	LBL-020	LBL-020	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-004	LBL-004	MR	LBL-005	LBL-005	MR
1-37	MR	LBL-001	LBL-001	LBL-001	MR	MR	MR	MR	LBL-020	LBL-020	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-004	LBL-004	MR	LBL-005	LBL-005	MR
1-38	MR	MR	MR	MR	LBL-001	LBL-023	LBL-023	LBL-023	MR	MR	MR	LBL-025	LBL-024	LBL-024	LBL-020	LBL-020	LBL-020	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-004	MR	MR	MR
1-39	MR	MR	MR	MR	LBL-023	LBL-023	LBL-023	LBL-023	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-40	MR	MR	MR	MR	LBL-023	LBL-023	LBL-023	LBL-023	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-41	MR	MR	MR	MR	LBL-023	LBL-023	LBL-023	LBL-023	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-42	MR	LBL-020	LBL-020	LBL-020	MR	MR	MR	MR	LBL-020	LBL-020	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	LBL-003	MR	LBL-009	LBL-009	MR
1-43	MR	LBL-020	LBL-020	LBL-020	MR	MR	MR	MR	LBL-020	LBL-020	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	LBL-003	MR	LBL-009	LBL-009	MR
1-44	MR	LBL-020	LBL-020	LBL-020	MR	MR	MR	MR	LBL-020	LBL-020	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	LBL-003	MR	LBL-009	LBL-009	MR
1-45	MR	MR	MR	MR	LBL-025	MR	MR	MR	MR	MR	MR	LBL-025	LBL-024	LBL-024	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-46	MR	MR	MR	MR	LBL-024	MR	MR	MR	MR	MR	MR	LBL-024	LBL-024	LBL-024	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-47	MR	MR	MR	MR	LBL-024	MR	MR	MR	MR	MR	MR	LBL-024	LBL-024	LBL-024	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-48	MR	MR	MR	MR	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-020	LBL-020	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-49	MR	MR	MR	MR	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-020	LBL-020	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-50	MR	MR	MR	MR	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-020	LBL-020	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-51	MR	MR	MR	MR	LBL-020	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-52	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-53	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-54	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-55	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-56	LBL-058	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-57	LBL-058	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-58	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-59	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-60	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-61	MR	LBL-004	LBL-004	LBL-004	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-62	MR	LBL-004	LBL-004	LBL-004	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-63	MR	MR	MR	MR	LBL-004	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-64	MR	LBL-005	LBL-005	LBL-005	MR	MR	MR	MR	LBL-009	LBL-009	LBL-009	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-65	MR	LBL-005	LBL-005	LBL-005	MR	MR	MR	MR	LBL-009	LBL-009	LBL-009	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-66	MR	MR	MR	MR	LBL-005	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR

1-01 to 1-33, 2-01 to 2-33

	2-01	2-02	2-03	2-04	2-05	2-06	2-07	2-08	2-09	2-10	2-11	2-12	2-13	2-14	2-15	2-16	2-17	2-18	2-19	2-20	2-21	2-22	2-23	2-24	2-25	2-26	2-27	2-28	2-29	2-30	2-31	2-32	2-33
1-01	LBL-047	LBL-042	LBL-042	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-02	LBL-051	LBL-042	LBL-042	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-03	LBL-047	LBL-042	LBL-042	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-04	MR	MR	MR	LBL-040	LBL-027	LBL-027	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-05	MR	MR	MR	LBL-031	LBL-027	LBL-027	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-06	MR	MR	MR	LBL-031	LBL-027	LBL-027	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-07	MR	MR	MR	MR	MR	MR		LBL-030	LBL-030	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-08	MR	MR	MR	MR	MR	MR		LBL-030	LBL-030	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-09	MR	MR	MR	MR	MR	MR	MR	MR	LBL-027	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-10	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-060	LBL-060	LBL-060	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-060	LBL-060	LBL-060	LBL-054	LBL-060	LBL-054	MR	MR	MR	MR
1-11	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR
1-12	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR
1-13	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR
1-14	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR
1-15	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR
1-16	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	LBL-002	LBL-002	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-17	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-075	LBL-075	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-18	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-075	LBL-075	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-19	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-20	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-21	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-063	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	LBL-067	LBL-067	MR	MR	MR	MR	MR	MR	MR	MR
1-22	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-063	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	LBL-067	LBL-067	MR	MR	MR	MR	MR	MR	MR	MR
1-23	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-067	LBL-061	LBL-061	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-067	LBL-067	LBL-067	LBL-054	LBL-067	LBL-054	MR	MR	MR	MR
1-24	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-060	LBL-060	LBL-060	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-060	LBL-060	LBL-060	LBL-054	LBL-060	LBL-054	MR	MR	MR	MR
1-25	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-076	LBL-061	LBL-061	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-075	LBL-081	LBL-081	LBL-054	LBL-081	LBL-054	MR	MR	MR	MR
1-26	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-058	LBL-058	LBL-058	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-058	LBL-058	LBL-058	LBL-054	LBL-058	LBL-054	MR	MR	MR	MR
1-27	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-076	LBL-061	LBL-061	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-075	LBL-088	LBL-088	LBL-054	LBL-088	LBL-054	MR	MR	MR	MR
1-28	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-058	LBL-058	LBL-058	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-058	LBL-058	LBL-058	LBL-054	LBL-058	LBL-054	MR	MR	MR	MR
1-29	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-063	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	LBL-073	LBL-073	MR	MR	MR	MR	MR	MR	MR	MR
1-30	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-063	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	LBL-077	LBL-077	MR	MR	MR	MR	MR	MR	MR	MR
1-31	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-063	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	LBL-071	LBL-071	MR	MR	MR	MR	MR	MR	MR	MR
1-32	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-063	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	LBL-077	LBL-077	MR	MR	MR	MR	MR	MR	MR	MR
1-33	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-063	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	LBL-071	LBL-071	MR	MR	MR	MR	MR	MR	MR	MR

1-01 to 1-33, 2-34 to 2-66

	2-34	2-35	2-36	2-37	2-38	2-39	2-40	2-41	2-42	2-43	2-44	2-45	2-46	2-47	2-48	2-49	2-50	2-51	2-52	2-53	2-54	2-55	2-56	2-57	2-58	2-59	2-60	2-61	2-62	2-63	2-64	2-65	2-66
1-01	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-02	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-03	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-04	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-05	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-06	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-07	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-08	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-09	MR	MR	MR	MR	MR	LBL-010	LBL-003	LBL-003	LBL-003	LBL-003	LBL-003	LBL-018	LBL-015	LBL-015	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-10	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-11	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-12	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-13	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-14	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-15	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-16	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-17	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-18	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-19	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-20	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-21	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-22	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-23	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-24	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-25	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-26	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-27	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-28	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-29	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-30	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-31	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-32	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
1-33	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR																						

1-34 to 1-66, 2-01 to 2-33

[illegible]

1-34 to 1-66, 2-34 to 2-36

	2-34	2-35	2-36	2-37	2-38	2-39	2-40	2-41	2-42	2-43	2-44	2-45	2-46	2-47	2-48	2-49	2-50	2-51	2-52	2-53	2-54	2-55	2-56	2-57	2-58	2-59	2-60	2-61	2-62	2-63	2-64	2-65	2-66	
1-34	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-058	LBL-058	MR	MR	LBL-058	LBL-058	LBL-058	LBL-058	LBL-057	MR	MR	MR	MR	MR	MR	
1-35	MR	LBL-001	LBL-113	LBL-113	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-004	LBL-004	MR	LBL-005	LBL-005	MR	
1-36	MR	LBL-001	LBL-113	LBL-113	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-004	LBL-004	MR	LBL-005	LBL-005	MR	
1-37	MR	LBL-001	LBL-113	LBL-113	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-004	LBL-004	MR	LBL-005	LBL-005	MR	
1-38	MR	MR	MR	MR	MR	LBL-113	LBL-010	LBL-003	LBL-003	MR	MR	MR	LBL-018	LBL-015	LBL-015	LBL-037	LBL-017	LBL-017	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-39	MR	MR	MR	MR	MR	LBL-010	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-40	MR	MR	MR	MR	MR	LBL-010	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-41	MR	MR	MR	MR	MR	LBL-010	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-42	MR	LBL-020	LBL-118	LBL-118	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	LBL-003	MR	LBL-009	LBL-009	MR
1-43	MR	LBL-020	LBL-118	LBL-118	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	LBL-003	MR	LBL-009	LBL-009	MR
1-44	MR	LBL-020	LBL-118	LBL-118	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	LBL-003	MR	LBL-009	LBL-009	MR
1-45	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-018	LBL-015	LBL-015	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-46	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-018	LBL-015	LBL-015	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-47	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-018	LBL-015	LBL-015	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-48	MR	MR	MR	MR	LBL-118	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-020	LBL-017	LBL-017	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-49	MR	MR	MR	MR	LBL-118	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-020	LBL-017	LBL-017	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-50	MR	MR	MR	MR	LBL-118	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-020	LBL-017	LBL-017	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-51	MR	MR	MR	MR	LBL-118	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-52	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-53	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-54	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-55	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-56	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-57	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-58	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-59	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-60	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-61	MR	LBL-004	LBL-008	LBL-008	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-62	MR	LBL-004	LBL-008	LBL-008	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
1-63	MR	MR	MR	MR	LBL-008	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR				

2-01 to 2-33, 2-01 to 2-33

	2-01	2-02	2-03	2-04	2-05	2-06	2-07	2-08	2-09	2-10	2-11	2-12	2-13	2-14	2-15	2-16	2-17	2-18	2-19	2-20	2-21	2-22	2-23	2-24	2-25	2-26	2-27	2-28	2-29	2-30	2-31	2-32	2-33
2-01	LBL-001	LBL-042	LBL-042	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-02	LBL-042	LBL-042	LBL-042	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-03	LBL-042	LBL-042	LBL-042	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-04	MR	MR	MR	LBL-050	LBL-027	LBL-027	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-05	MR	MR	MR	LBL-027	LBL-027	LBL-027	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-06	MR	MR	MR	LBL-027	LBL-027	LBL-027	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-07	MR	MR	MR	MR	MR	MR	LBL-030	LBL-030	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-08	MR	MR	MR	MR	MR	MR	LBL-030	LBL-030	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-09	MR	MR	MR	MR	MR	MR	MR	MR	LBL-027	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-10	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-076	LBL-061	LBL-061	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-075	LBL-076	LBL-076	LBL-054	LBL-076	LBL-054	MR	MR	MR	MR	MR
2-11	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-061	LBL-061	LBL-061	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-061	LBL-061	LBL-061	LBL-054	LBL-061	LBL-054	MR	MR	MR	MR	MR
2-12	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-061	LBL-061	LBL-061	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-061	LBL-061	LBL-061	LBL-054	LBL-061	LBL-054	MR	MR	MR	MR	MR
2-13	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-063	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	LBL-063	LBL-063	MR	MR	MR	MR	MR	MR	MR	MR	MR	
2-14	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	
2-15	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	
2-16	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-17	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-075	LBL-075	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-18	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-075	LBL-075	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-19	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	LBL-094	LBL-094	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-20	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	LBL-094	LBL-094	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-21	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-063	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	LBL-077	LBL-077	MR	MR	MR	MR	MR	MR	MR	MR	
2-22	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-063	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	LBL-077	LBL-077	MR	MR	MR	MR	MR	MR	MR	MR	
2-23	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-24	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-25	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-26	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-27	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-28	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-29	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-30	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-31	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-32	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-33	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR

2-01 to 2-33, 2-34 to 2-66

	2-34	2-35	2-36	2-37	2-38	2-39	2-40	2-41	2-42	2-43	2-44	2-45	2-46	2-47	2-48	2-49	2-50	2-51	2-52	2-53	2-54	2-55	2-56	2-57	2-58	2-59	2-60	2-61	2-62	2-63	2-64	2-65	2-66
2-01	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-02	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-03	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-04	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-05	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-06	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-07	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-08	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-09	MR	MR	MR	MR	MR	LBL-010	LBL-003	LBL-003	LBL-003	LBL-003	LBL-003	LBL-018	LBL-015	LBL-015	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-10	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-11	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-12	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-13	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-14	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-15	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-16	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-17	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-18	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-19	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-20	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-21	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-22	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-23	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-24	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-25	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-26	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-27	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-28	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-29	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-30	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-31	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-32	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-33	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR</																						

2-34 to 2-66, 2-01 to 2-33

	2-01	2-02	2-03	2-04	2-05	2-06	2-07	2-08	2-09	2-10	2-11	2-12	2-13	2-14	2-15	2-16	2-17	2-18	2-19	2-20	2-21	2-22	2-23	2-24	2-25	2-26	2-27	2-28	2-29	2-30	2-31	2-32	2-33
2-34	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-054	LBL-054	LBL-054	LBL-054	MR	MR	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-35	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-36	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-37	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-38	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-39	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-010	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-40	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-41	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-42	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-43	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-44	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-45	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-018	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-46	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-015	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-47	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-015	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-48	MR	MR	MR	MR	MR	MR	MR	LBL-030	LBL-030	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-49	MR	MR	MR	MR	MR	MR	MR	LBL-017	LBL-017	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-50	MR	MR	MR	MR	MR	MR	MR	LBL-017	LBL-017	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-51	LBL-003	LBL-003	LBL-003	LBL-003	LBL-003	LBL-003	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-52	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR	LBL-067	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-53	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR	LBL-067	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-54	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-057	LBL-057	LBL-057	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-057	LBL-057	LBL-057	LBL-054	LBL-057	LBL-054	MR	MR	MR	MR	MR
2-55	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-057	LBL-057	LBL-057	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-057	LBL-057	LBL-057	LBL-054	LBL-057	LBL-054	MR	MR	MR	MR	MR
2-56	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR	LBL-062	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-57	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR	LBL-062	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-58	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-069	LBL-069	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-59	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-069	LBL-069	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-60	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-057	LBL-002	LBL-002	LBL-002	MR	MR	LBL-057	LBL-057	LBL-057	LBL-057	LBL-057	MR	MR	MR	MR	MR	MR	LBL-057	LBL-057	LBL-057	LBL-057
2-61	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-62	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-63	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-64	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-65	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-66	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR



2-34 to 2-66, 2-34 to 2-66

	2-34	2-35	2-36	2-37	2-38	2-39	2-40	2-41	2-42	2-43	2-44	2-45	2-46	2-47	2-48	2-49	2-50	2-51	2-52	2-53	2-54	2-55	2-56	2-57	2-58	2-59	2-60	2-61	2-62	2-63	2-64	2-65	2-66
2-34	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-054	LBL-054	MR	MR	LBL-054	LBL-054	LBL-054	LBL-054	LBL-054	MR	MR	MR	MR	MR	MR
2-35	MR	LBL-001	LBL-113	LBL-113	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-004	LBL-004	MR	LBL-005	LBL-005	MR
2-36	MR	LBL-113	LBL-113	LBL-113	MR	MR	MR	MR	LBL-006	LBL-006	LBL-006	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-008	LBL-008	MR	LBL-005	LBL-005	MR
2-37	MR	LBL-113	LBL-113	LBL-113	MR	MR	MR	MR	LBL-006	LBL-006	LBL-006	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-008	LBL-008	MR	LBL-005	LBL-005	MR
2-38	MR	MR	MR	MR	LBL-113	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-120	LBL-119	LBL-119	LBL-006	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-39	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-40	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-41	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-42	MR	LBL-003	LBL-006	LBL-006	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-43	MR	LBL-003	LBL-006	LBL-006	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-44	MR	LBL-003	LBL-006	LBL-006	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-45	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-46	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-47	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-48	MR	MR	MR	MR	LBL-120	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-49	MR	MR	MR	MR	LBL-119	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-50	MR	MR	MR	MR	LBL-119	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-51	MR	MR	MR	MR	LBL-006	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-52	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-53	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-54	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-55	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-56	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-57	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-58	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-59	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-60	LBL-054	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-61	MR	LBL-004	LBL-008	LBL-008	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-62	MR	LBL-004	LBL-008	LBL-008	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-63	MR	MR	MR	MR	LBL-008	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-64	MR	LBL-005	LBL-005	LBL-005	MR	MR	MR	MR	LBL-009	LBL-009	LBL-009	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-65	MR	LBL-005	LBL-005	LBL-005	MR	MR	MR	MR	LBL-009	LBL-009	LBL-009	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
2-66	MR	MR	MR	MR	LBL-005	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR

3-01 to 3-33, 3-01 to 3-33

	3-01	3-02	3-03	3-04	3-05	3-06	3-07	3-08	3-09	3-10	3-11	3-12	3-13	3-14	3-15	3-16	3-17	3-18	3-19	3-20	3-21	3-22	3-23	3-24	3-25	3-26	3-27	3-28	3-29	3-30	3-31	3-32	3-33
3-01	LBL-001	LBL-048	LBL-048	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-02	LBL-048	LBL-048	LBL-048	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-03	LBL-048	LBL-048	LBL-048	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-04	MR	MR	MR	LBL-001	LBL-045	LBL-045	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-05	MR	MR	MR	LBL-045	LBL-045	LBL-045	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-06	MR	MR	MR	LBL-045	LBL-045	LBL-045	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-07	MR	MR	MR	MR	MR	MR	LBL-041	LBL-041	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-08	MR	MR	MR	MR	MR	MR	LBL-041	LBL-041	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-09	MR	MR	MR	MR	MR	MR	MR	MR	LBL-041	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-10	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-086	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-086	LBL-086	LBL-086	LBL-078	LBL-086	LBL-078	MR	MR	MR	MR
3-11	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-053	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-053	LBL-053	LBL-053	LBL-053	LBL-053	LBL-053	MR	MR	MR	MR
3-12	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-053	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-053	LBL-053	LBL-053	LBL-053	LBL-053	LBL-053	MR	MR	MR	MR
3-13	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-065	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	LBL-065	LBL-065	MR	MR	MR	MR	MR	MR	MR	MR	
3-14	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	
3-15	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	
3-16	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	LBL-002	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-17	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-102	LBL-102	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-18	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-102	LBL-102	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-19	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-20	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-21	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-065	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	LBL-095	LBL-095	MR	MR	MR	MR	MR	MR	MR	
3-22	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-065	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	LBL-095	LBL-095	MR	MR	MR	MR	MR	MR	MR	
3-23	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-086	LBL-053	LBL-053	MR	MR	MR	LBL-002	MR	MR	MR	MR	MR	MR	MR	LBL-095	LBL-095	LBL-095	LBL-078	LBL-095	LBL-078	MR	MR	MR	MR
3-24	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-086	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-095	LBL-096	LBL-096	LBL-078	LBL-096	LBL-078	MR	MR	MR	MR
3-25	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-086	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-095	LBL-096	LBL-001	LBL-078	LBL-001	LBL-078	MR	MR	MR	MR
3-26	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-078	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-078	LBL-078	LBL-078	LBL-078	LBL-078	LBL-078	MR	MR	MR	MR
3-27	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-086	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-095	LBL-096	LBL-001	LBL-078	LBL-001	LBL-078	MR	MR	MR	MR
3-28	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-078	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-078	LBL-078	LBL-078	LBL-078	LBL-078	LBL-078	MR	MR	MR	MR
3-29	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-065	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	LBL-070	LBL-070	MR	MR	MR	MR	MR	MR	MR	
3-30	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-065	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	LBL-095	LBL-095	MR	MR	MR	MR	MR	MR	MR	
3-31	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-065	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	LBL-092	LBL-092	MR	MR	MR	MR	MR	MR	MR	
3-32	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-065	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	LBL-095	LBL-095	MR	MR	MR	MR	MR	MR	MR	
3-33	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-065	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	LBL-070	LBL-070	MR	MR	MR	MR	MR	MR	MR	

3-01 to 3-33, 3-34 to 3-66

	3-34	3-35	3-36	3-37	3-38	3-39	3-40	3-41	3-42	3-43	3-44	3-45	3-46	3-47	3-48	3-49	3-50	3-51	3-52	3-53	3-54	3-55	3-56	3-57	3-58	3-59	3-60	3-61	3-62	3-63	3-64	3-65	3-66
3-01	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-02	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-03	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-04	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-05	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-06	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-07	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-035	LBL-021	LBL-021	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-08	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-035	LBL-021	LBL-021	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-09	MR	MR	MR	MR	MR	LBL-013	LBL-011	LBL-011	LBL-017	LBL-003	LBL-003	LBL-028	LBL-022	LBL-022	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-10	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-11	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-12	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-13	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-053	MR	MR	MR	MR	MR	MR
3-14	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-15	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-16	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-002	LBL-002	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-17	LBL-070	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-18	LBL-070	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-19	LBL-070	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-20	LBL-070	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-21	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-22	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-23	LBL-070	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-063	LBL-063	LBL-053	LBL-053	LBL-061	LBL-061	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-24	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-25	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-26	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-27	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-28	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-29	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-30	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-31	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-32	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR
3-33	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR

3-34 to 3-66, 3-01 to 3-33

[illegible]

3-34 to 3-66, 3-34 to 3-66

	3-34	3-35	3-36	3-37	3-38	3-39	3-40	3-41	3-42	3-43	3-44	3-45	3-46	3-47	3-48	3-49	3-50	3-51	3-52	3-53	3-54	3-55	3-56	3-57	3-58	3-59	3-60	3-61	3-62	3-63	3-64	3-65	3-66	
3-34	LBL-070	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-063	LBL-063	MR	MR	LBL-061	LBL-061	LBL-068	LBL-068	LBL-053	MR	MR	MR	MR	MR	MR	
3-35	MR	LBL-001	LBL-115	LBL-115	MR	MR	MR	MR	LBL-017	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-116	LBL-004	MR	LBL-005	LBL-005	MR	
3-36	MR	LBL-115	LBL-115	LBL-115	MR	MR	MR	MR	LBL-119	LBL-006	LBL-006	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-121	LBL-008	MR	LBL-005	LBL-005	MR	
3-37	MR	LBL-115	LBL-115	LBL-115	MR	MR	MR	MR	LBL-119	LBL-006	LBL-006	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-121	LBL-008	MR	LBL-005	LBL-005	MR	
3-38	MR	MR	MR	MR	LBL-115	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-122	LBL-123	LBL-123	LBL-006	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-39	MR	MR	MR	MR	MR	LBL-013	LBL-011	LBL-011	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-40	MR	MR	MR	MR	MR	LBL-011	LBL-011	LBL-011	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-41	MR	MR	MR	MR	MR	LBL-011	LBL-011	LBL-011	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-42	MR	LBL-017	LBL-119	LBL-119	MR	MR	MR	MR	LBL-017	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-017	LBL-003	MR	LBL-009	LBL-009	MR	
3-43	MR	LBL-003	LBL-006	LBL-006	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	LBL-003	MR	LBL-009	LBL-009	MR	
3-44	MR	LBL-003	LBL-006	LBL-006	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	LBL-003	MR	LBL-009	LBL-009	MR	
3-45	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-028	LBL-022	LBL-022	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-46	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-022	LBL-022	LBL-022	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-47	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-022	LBL-022	LBL-022	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-48	MR	MR	MR	MR	LBL-122	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-035	LBL-021	LBL-021	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-49	MR	MR	MR	MR	LBL-123	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-021	LBL-021	LBL-021	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-50	MR	MR	MR	MR	LBL-123	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-021	LBL-021	LBL-021	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-51	MR	MR	MR	MR	LBL-006	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-52	LBL-063	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-063	LBL-063	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-53	LBL-063	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-063	LBL-063	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-54	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-55	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-053	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-56	LBL-061	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-061	LBL-061	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-57	LBL-061	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-061	LBL-061	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-58	LBL-068	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-59	LBL-068	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-60	LBL-053	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-61	MR	LBL-116	LBL-121	LBL-121	MR	MR	MR	MR	LBL-017	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-116	LBL-004	MR	LBL-007	LBL-007	MR
3-62	MR	LBL-004	LBL-008	LBL-008	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-004	LBL-004	MR	LBL-007	LBL-007	MR
3-63	MR	MR	MR	MR	LBL-008	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-003	LBL-003	LBL-003	LBL-003	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-64	MR	LBL-005	LBL-005	LBL-005	MR	MR	MR	MR	LBL-009	LBL-009	LBL-009	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-65	MR	LBL-005	LBL-005	LBL-005	MR	MR	MR	MR	LBL-009	LBL-009	LBL-009	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	
3-66	MR	MR	MR	MR	LBL-005	MR	MR	MR	MR	MR	MR	MR	MR	MR	LBL-009	LBL-009	LBL-009	LBL-009	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	MR	

## Labels

LBL-001 .....	49
LBL-002 .....	50
LBL-003 .....	51
LBL-004 .....	52
LBL-005 .....	53
LBL-006 .....	54
LBL-007 .....	55
LBL-008 .....	56
LBL-009 .....	57
LBL-010 .....	58
LBL-011 .....	59
LBL-012 .....	60
LBL-013 .....	61
LBL-014 .....	62
LBL-015 .....	63
LBL-016 .....	64
LBL-017 .....	65
LBL-018 .....	66
LBL-019 .....	67
LBL-020 .....	68
LBL-021 .....	69
LBL-022 .....	70
LBL-023 .....	71
LBL-024 .....	72
LBL-025 .....	73
LBL-026 .....	74
LBL-027 .....	75
LBL-028 .....	76
LBL-029 .....	77
LBL-030 .....	78
LBL-031 .....	79
LBL-032 .....	80
LBL-033 .....	81
LBL-034 .....	82
LBL-035 .....	83
LBL-036 .....	84
LBL-037 .....	85
LBL-038 .....	86
LBL-039 .....	87
LBL-040 .....	88
LBL-041 .....	89
LBL-042 .....	90
LBL-043 .....	91
LBL-044 .....	92
LBL-045 .....	93
LBL-046 .....	94
LBL-047 .....	95

LBL-048.....	96
LBL-049.....	97
LBL-050.....	98
LBL-051.....	99
LBL-052.....	100
LBL-053.....	101
LBL-054.....	102
LBL-055.....	103
LBL-056.....	104
LBL-057.....	105
LBL-058.....	106
LBL-059.....	107
LBL-060.....	108
LBL-061.....	109
LBL-062.....	110
LBL-063.....	111
LBL-064.....	112
LBL-065.....	113
LBL-066.....	114
LBL-067.....	115
LBL-068.....	116
LBL-069.....	117
LBL-070.....	118
LBL-071.....	119
LBL-072.....	120
LBL-073.....	121
LBL-074.....	122
LBL-075.....	123
LBL-076.....	124
LBL-077.....	125
LBL-078.....	126
LBL-079.....	127
LBL-080.....	128
LBL-081.....	129
LBL-082.....	130
LBL-083.....	131
LBL-084.....	132
LBL-085.....	133
LBL-086.....	134
LBL-087.....	135
LBL-088.....	136
LBL-089.....	137
LBL-090.....	138
LBL-091.....	139
LBL-092.....	140
LBL-093.....	141
LBL-094.....	142
LBL-095.....	143
LBL-096.....	144

<i>LBL-097</i> .....	145
<i>LBL-098</i> .....	146
<i>LBL-099</i> .....	147
<i>LBL-100</i> .....	148
<i>LBL-101</i> .....	149
<i>LBL-102</i> .....	150
<i>LBL-103</i> .....	151
<i>LBL-104</i> .....	152
<i>LBL-105</i> .....	153
<i>LBL-106</i> .....	154
<i>LBL-107</i> .....	155
<i>LBL-108</i> .....	156
<i>LBL-109</i> .....	157
<i>LBL-110</i> .....	158
<i>LBL-111</i> .....	159
<i>LBL-112</i> .....	160
<i>LBL-113</i> .....	161
<i>LBL-114</i> .....	162
<i>LBL-115</i> .....	163
<i>LBL-116</i> .....	164
<i>LBL-117</i> .....	165
<i>LBL-118</i> .....	166
<i>LBL-119</i> .....	167
<i>LBL-120</i> .....	168
<i>LBL-121</i> .....	169
<i>LBL-122</i> .....	170
<i>LBL-123</i> .....	171



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain lead codes and/or lead code combinations. Refer to the guide on page 11 for directions on how to generate a patient's lead code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg)
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.


**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

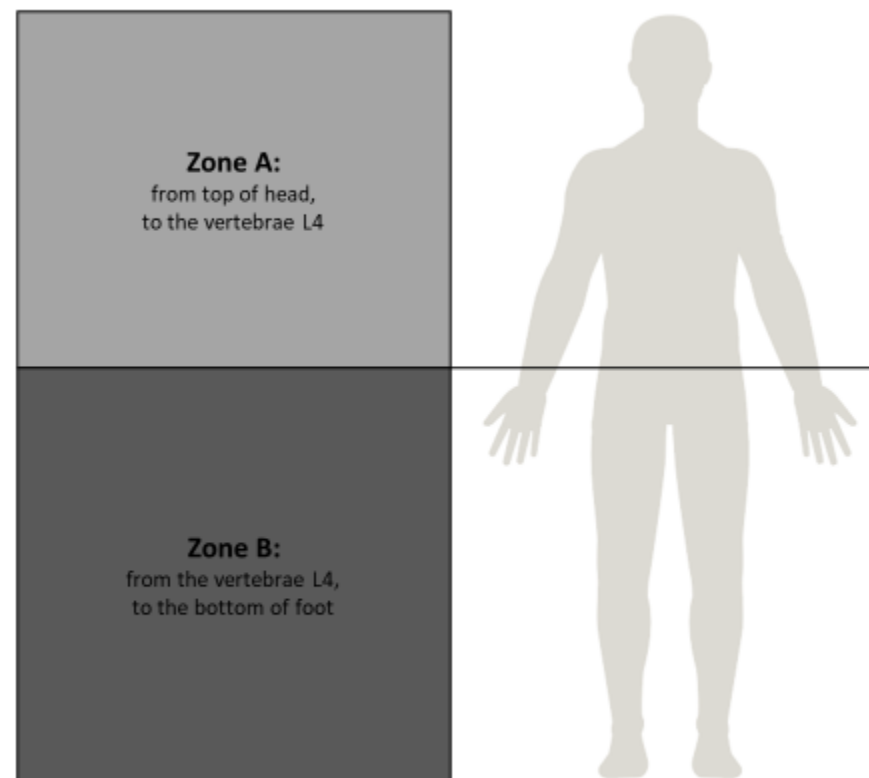


**Figure 2**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

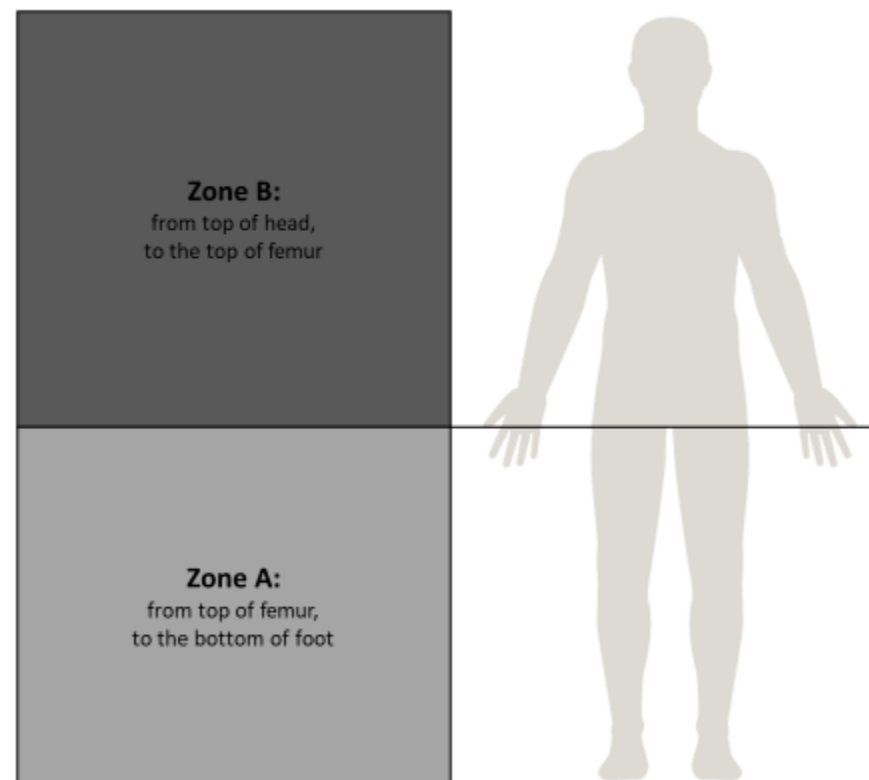


**Figure 3**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

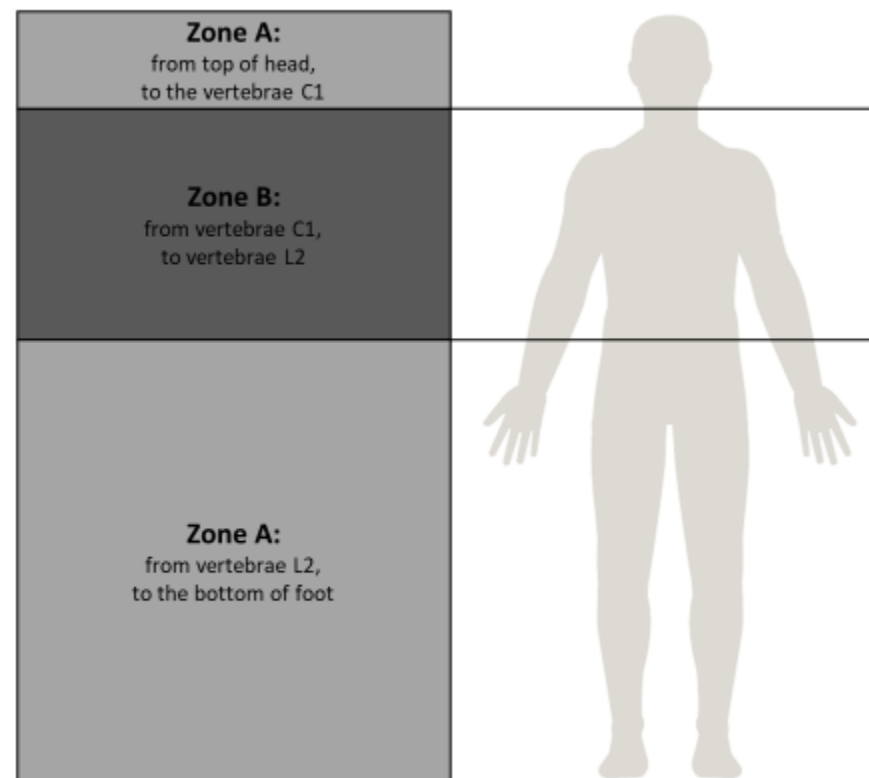


**Figure 4**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

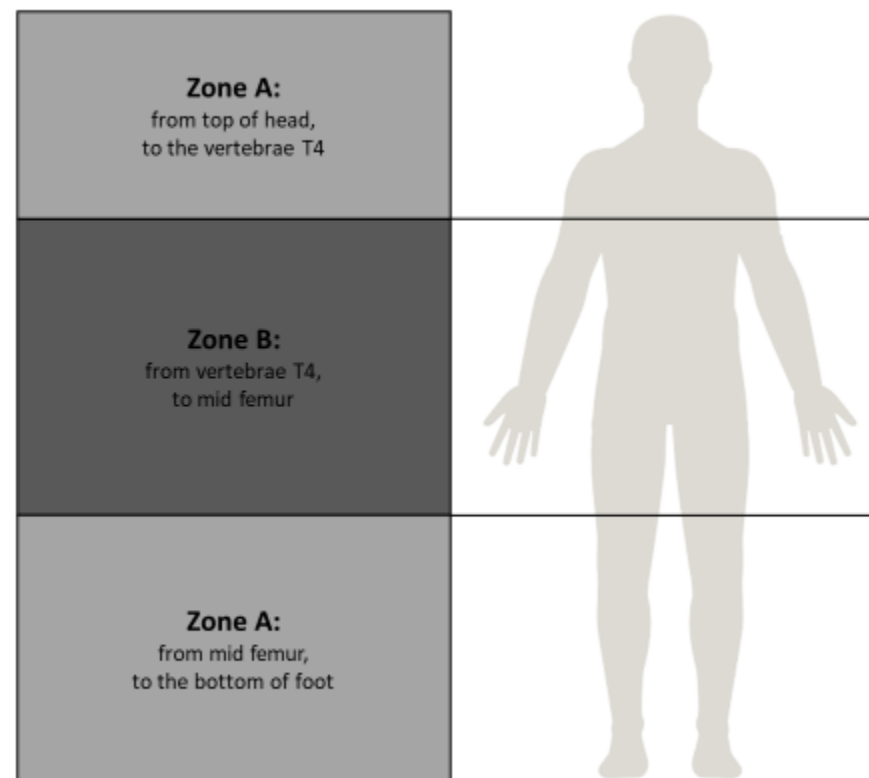
**Figure 5**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

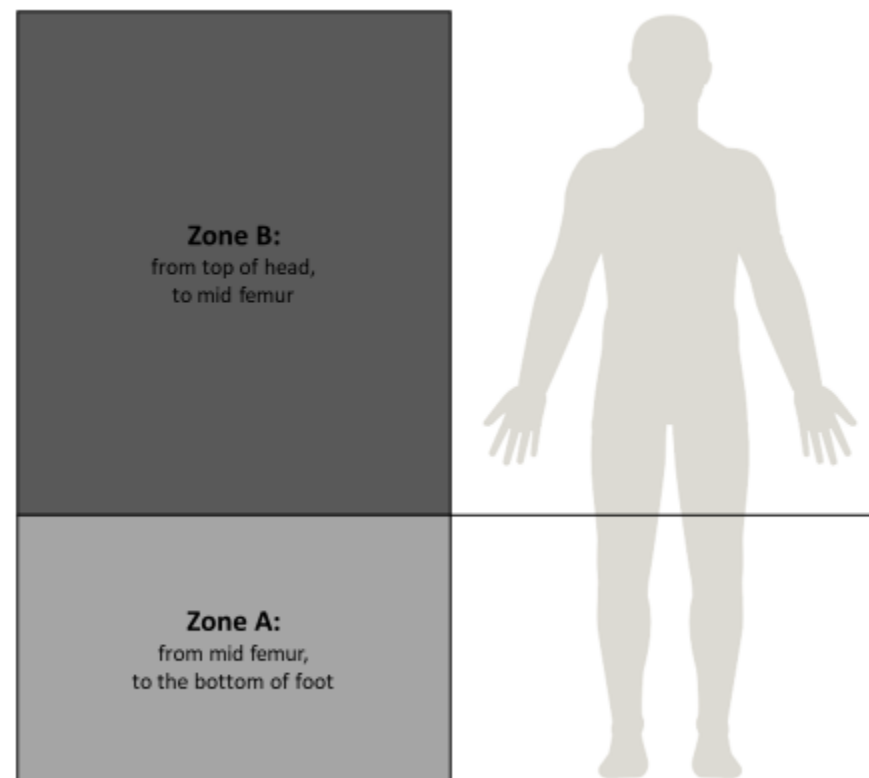


**Figure 6**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

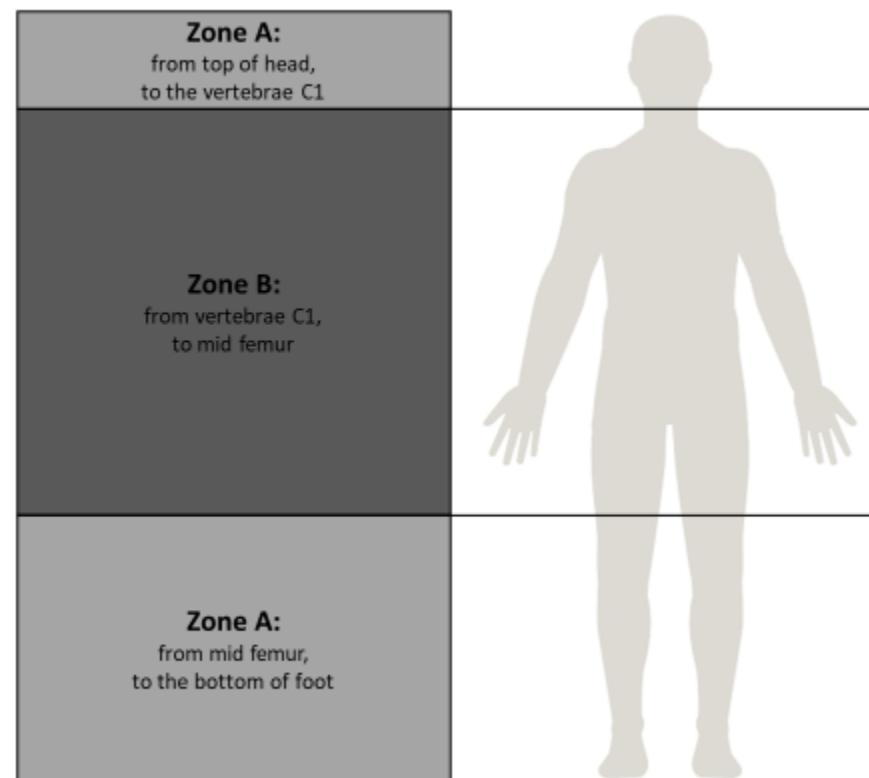


**Figure 7**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

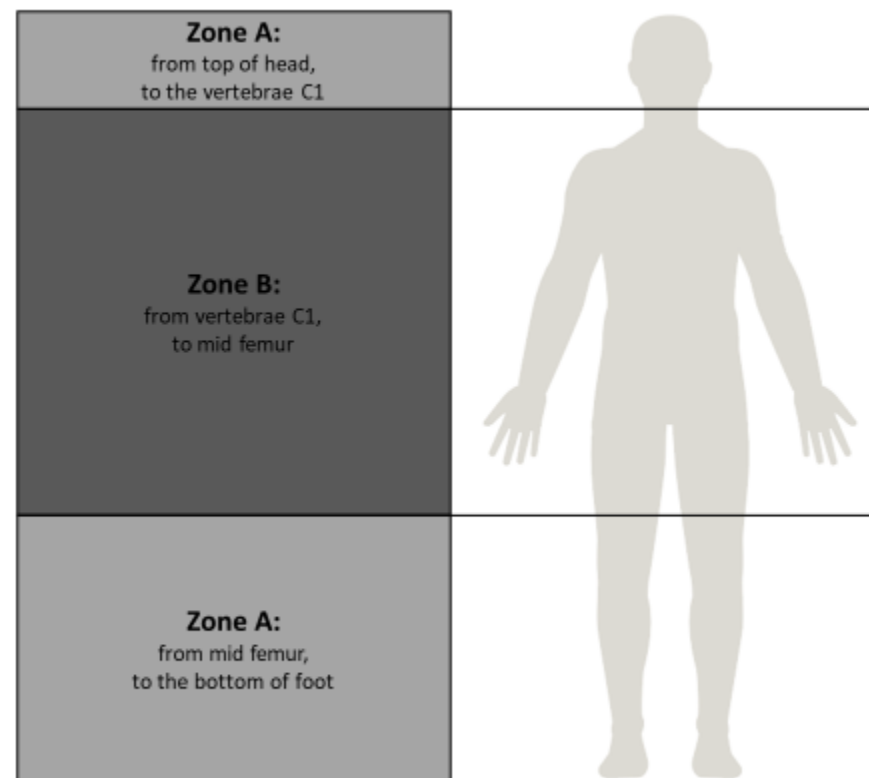**Figure 8**




**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

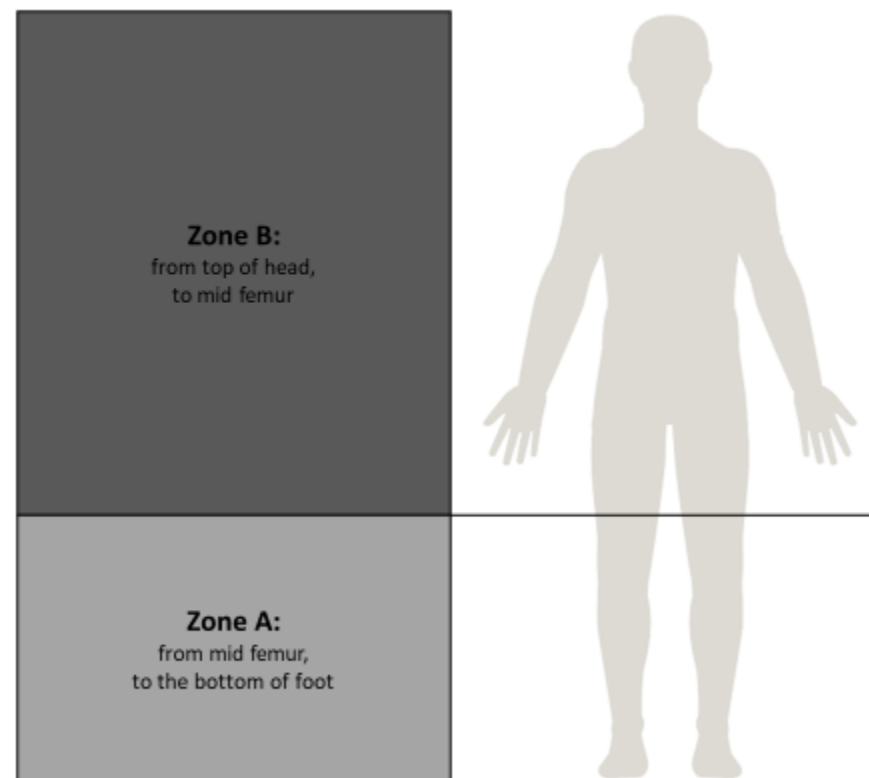

**Figure 9**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

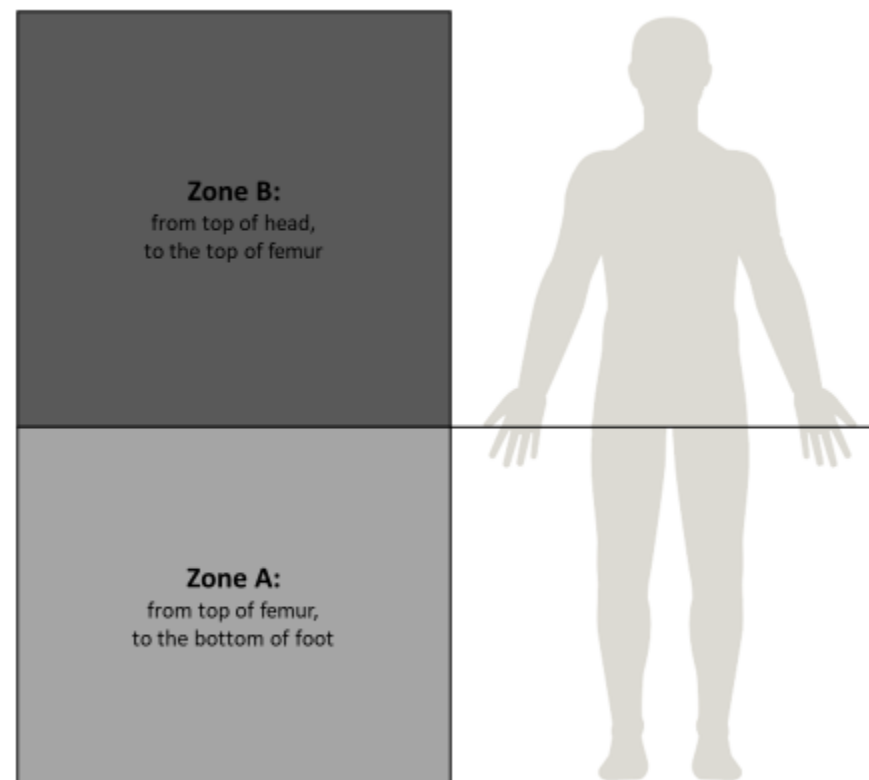


Figure 10

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

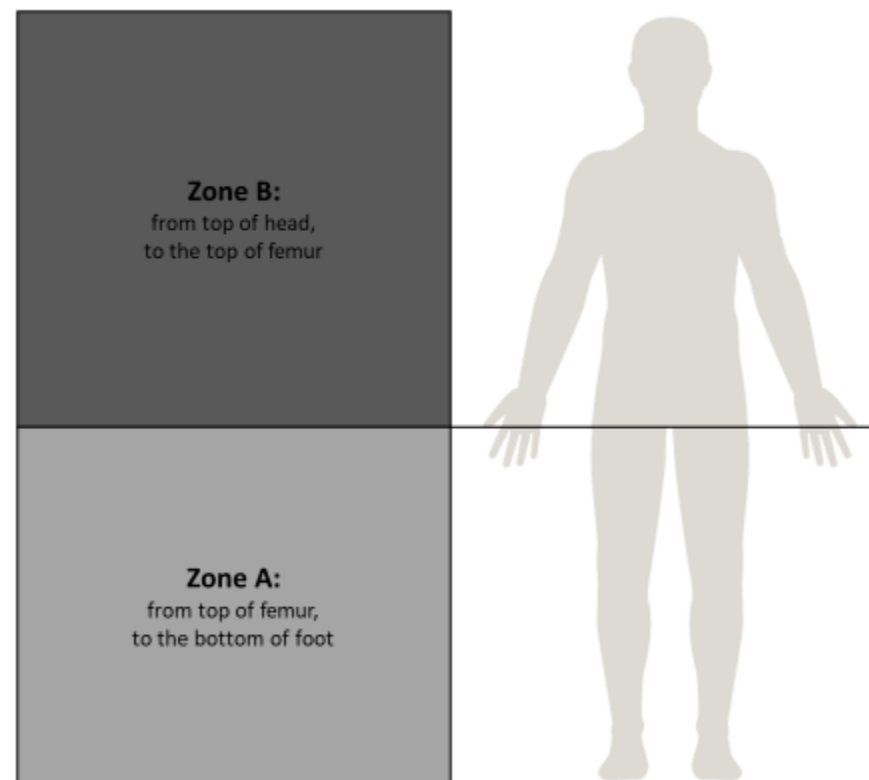


Figure 11

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

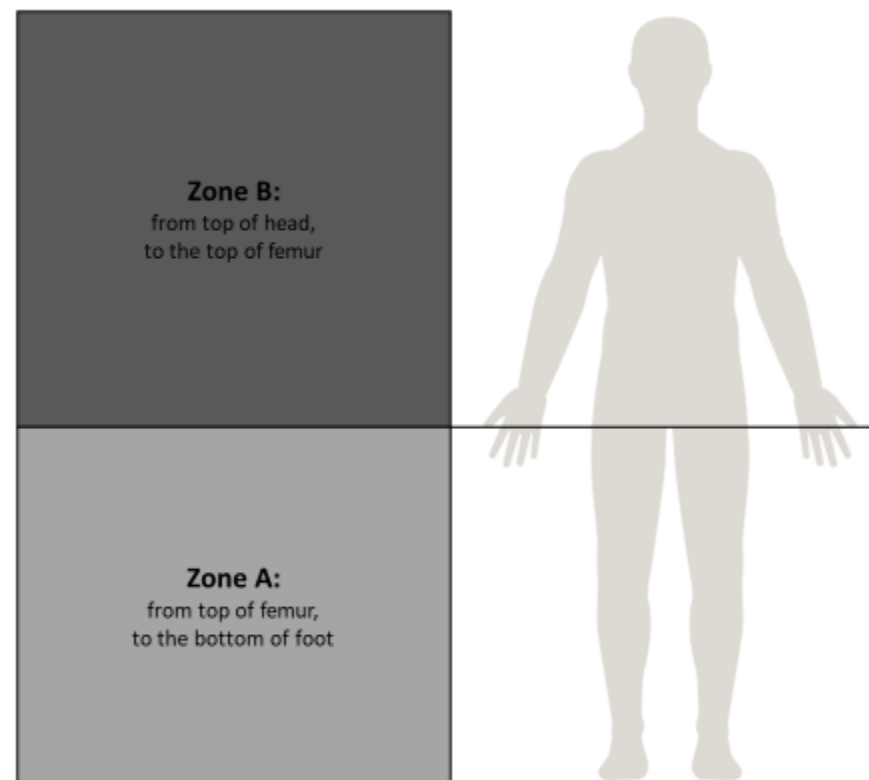


Figure 12

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

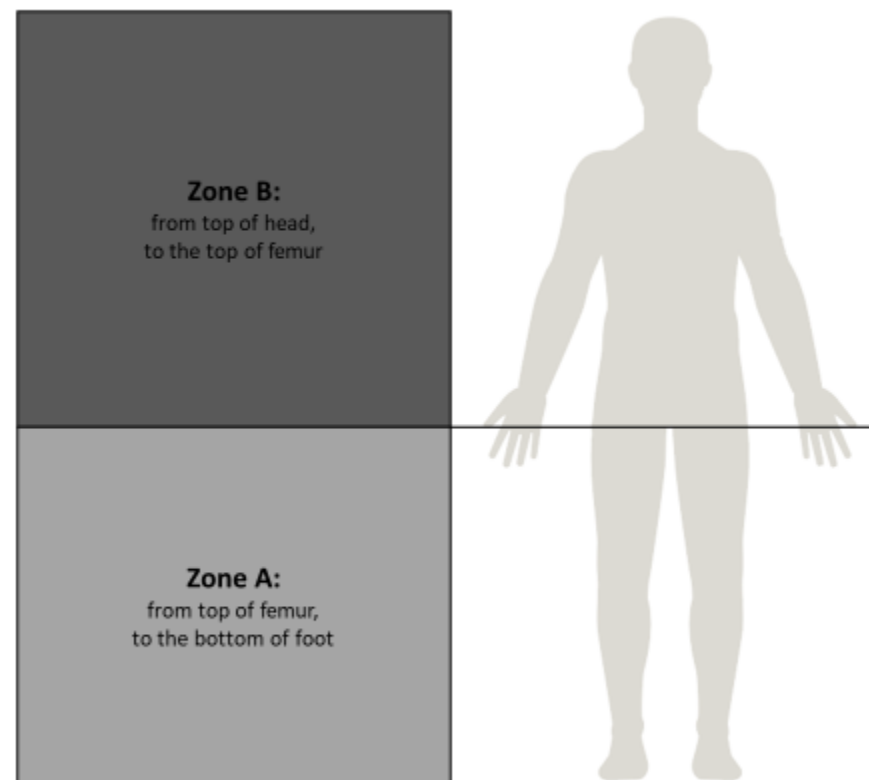


Figure 13

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

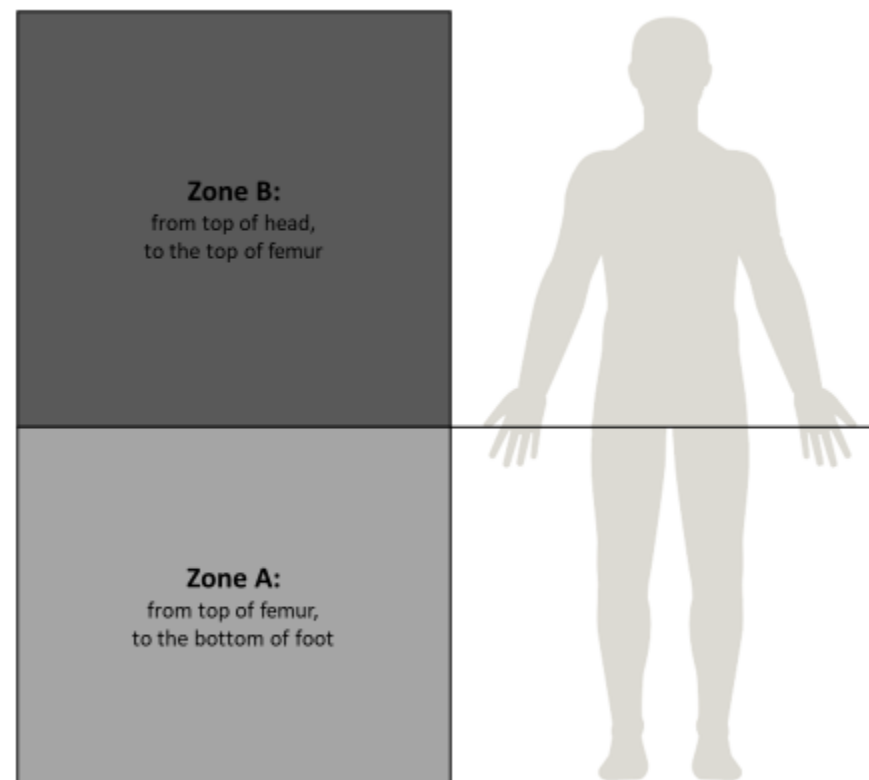


Figure 14

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

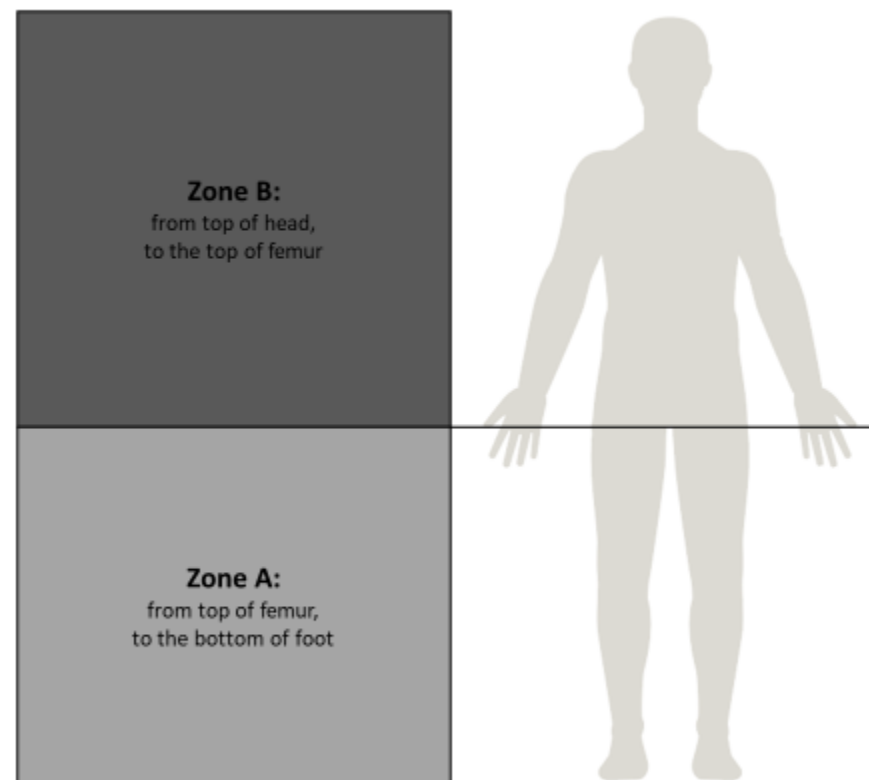


Figure 15



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

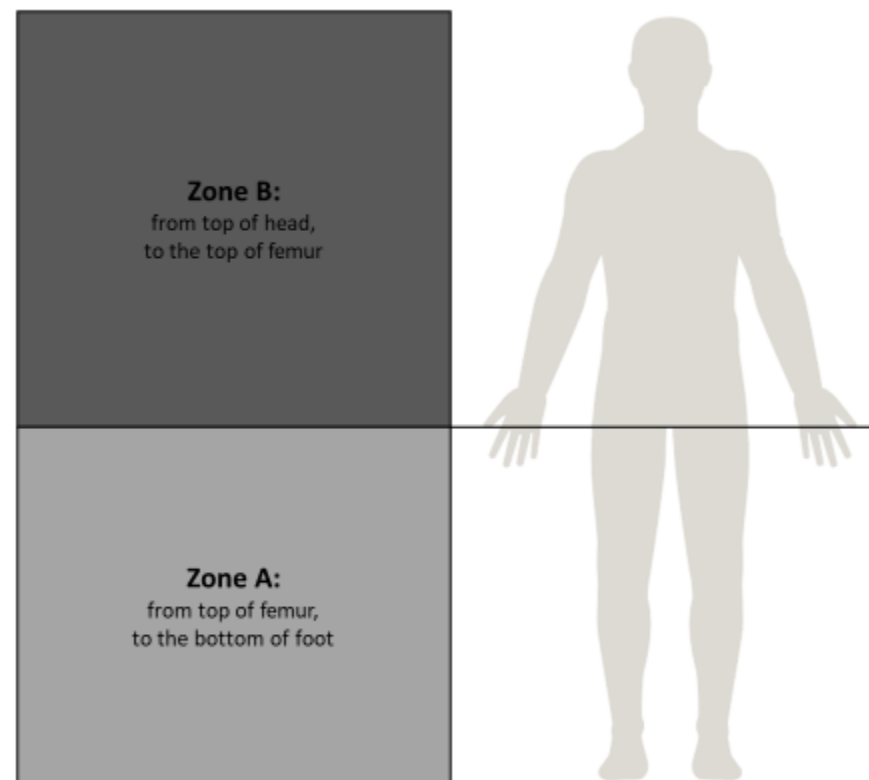


Figure 16



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

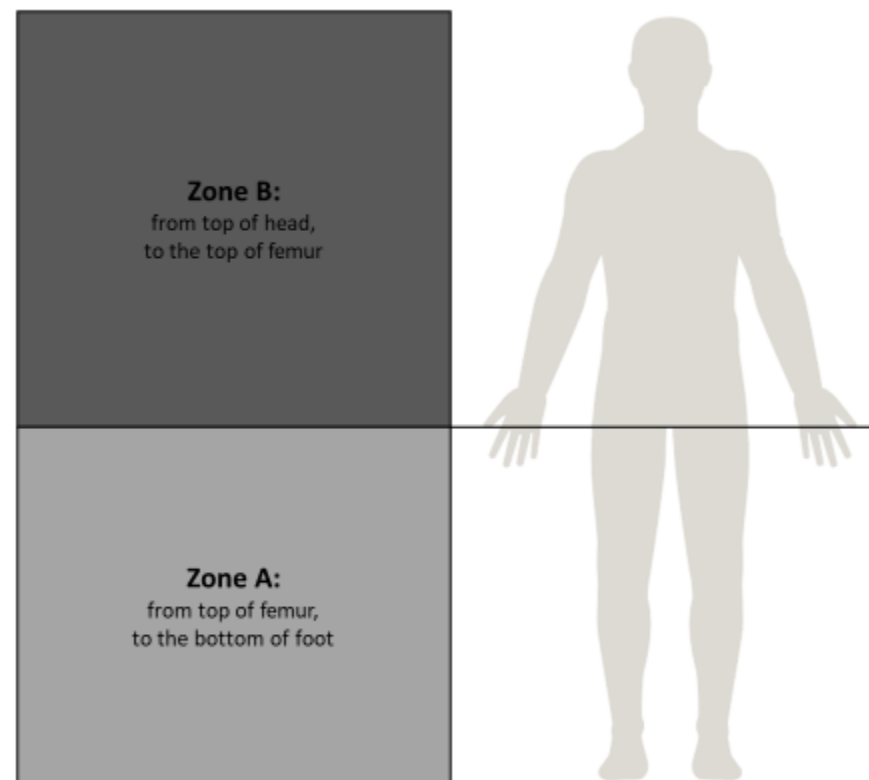


Figure 17

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

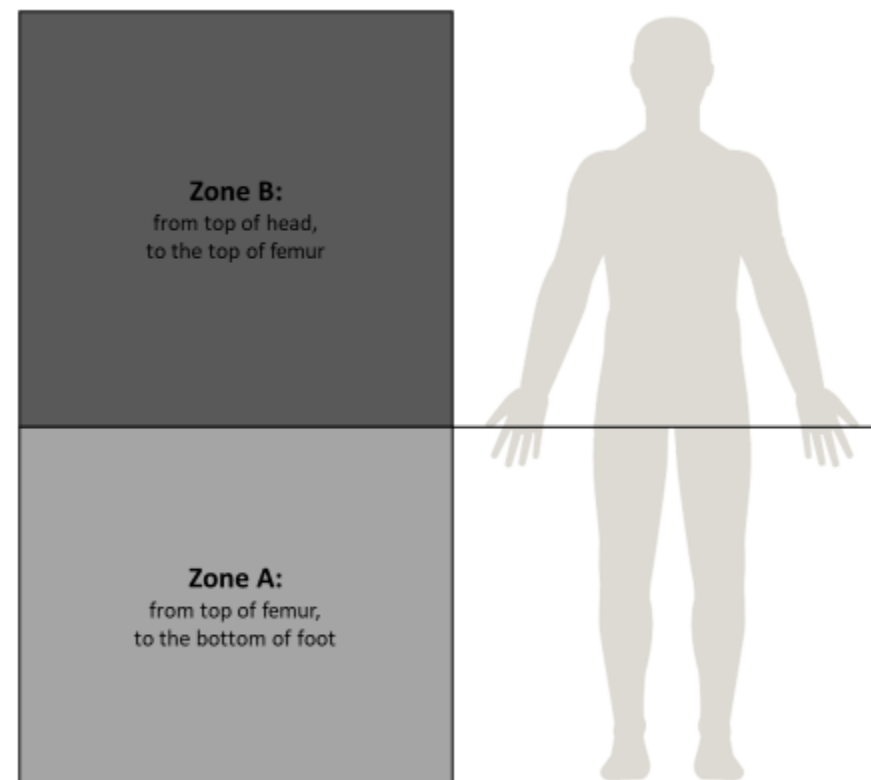


Figure 18

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

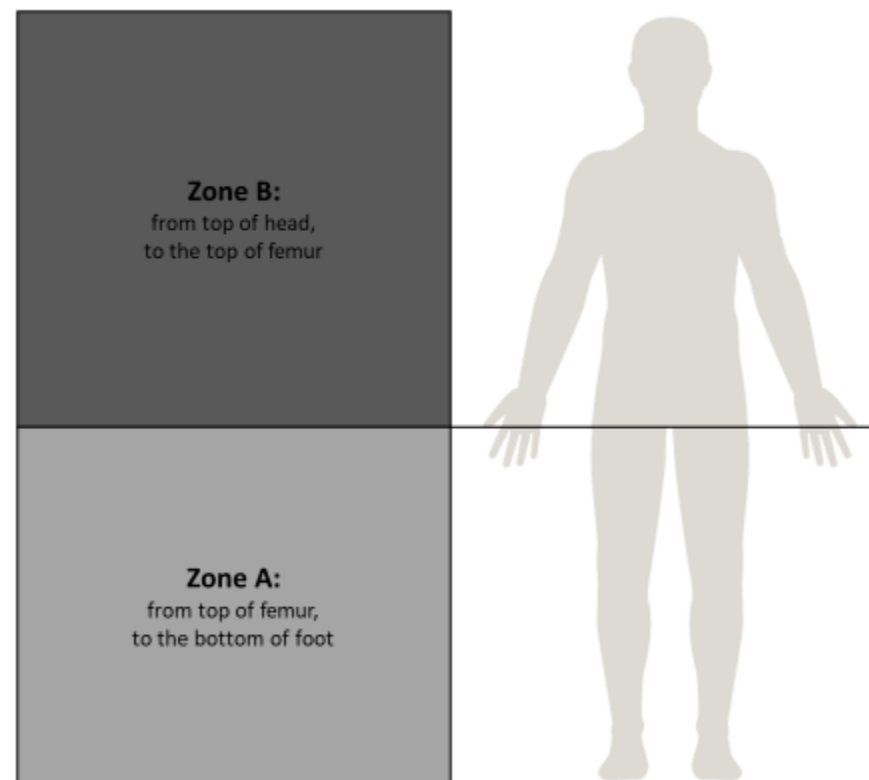


Figure 19

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

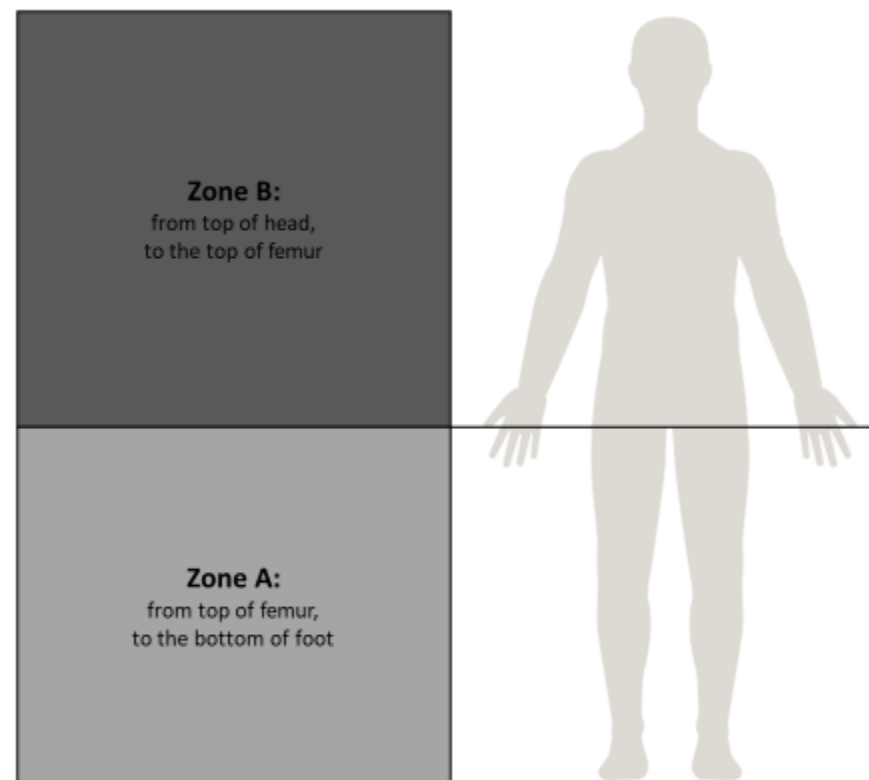


Figure 20

# MR Conditional



## MRI Safety Information

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq$ 2 W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

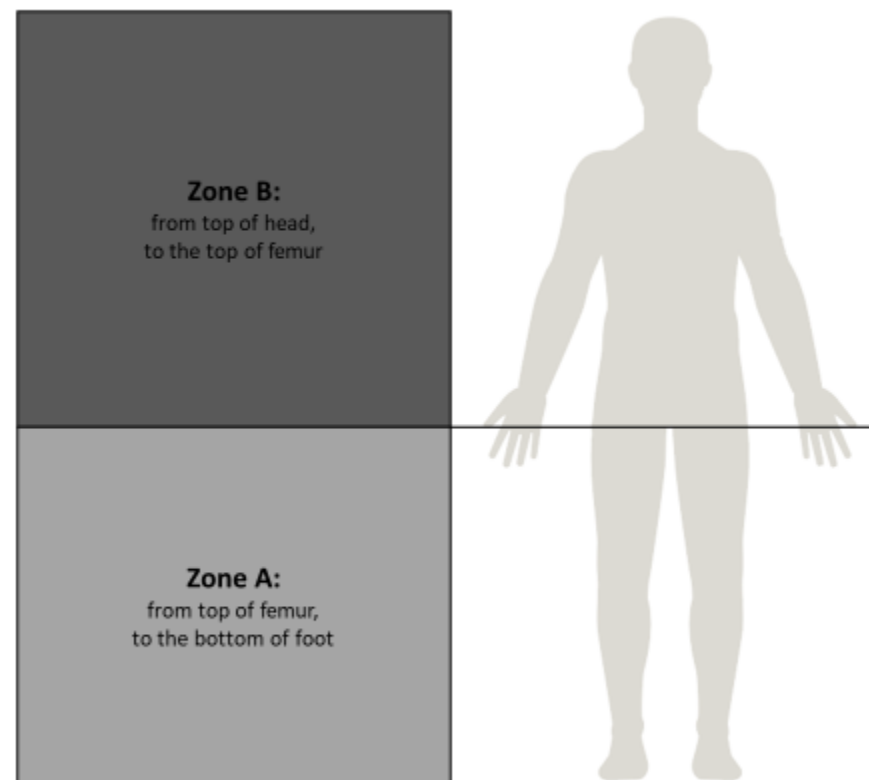


Figure 21

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

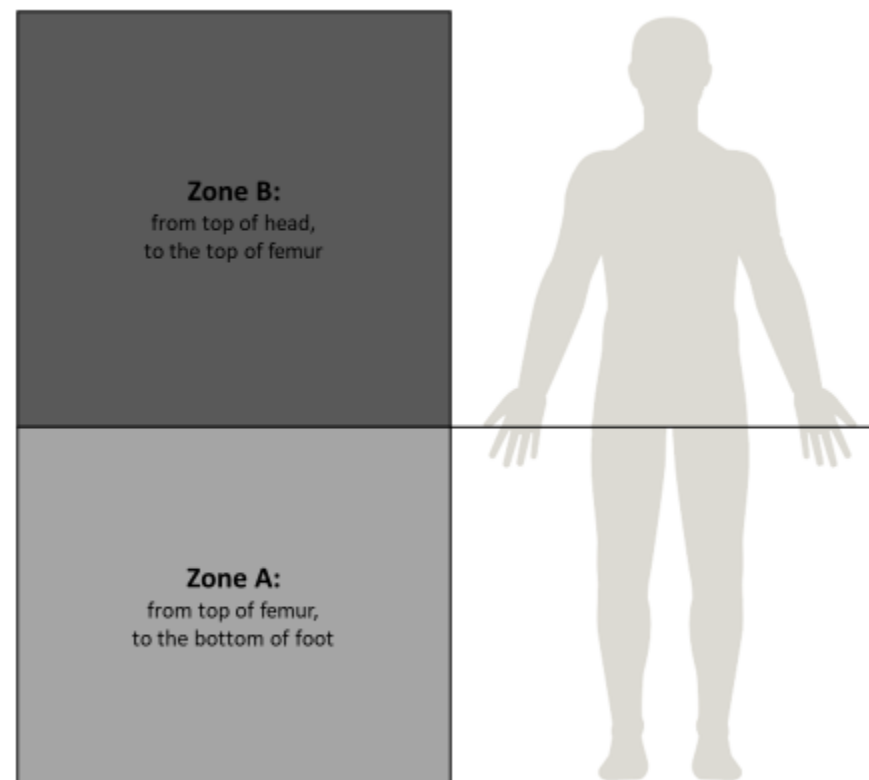


Figure 22

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

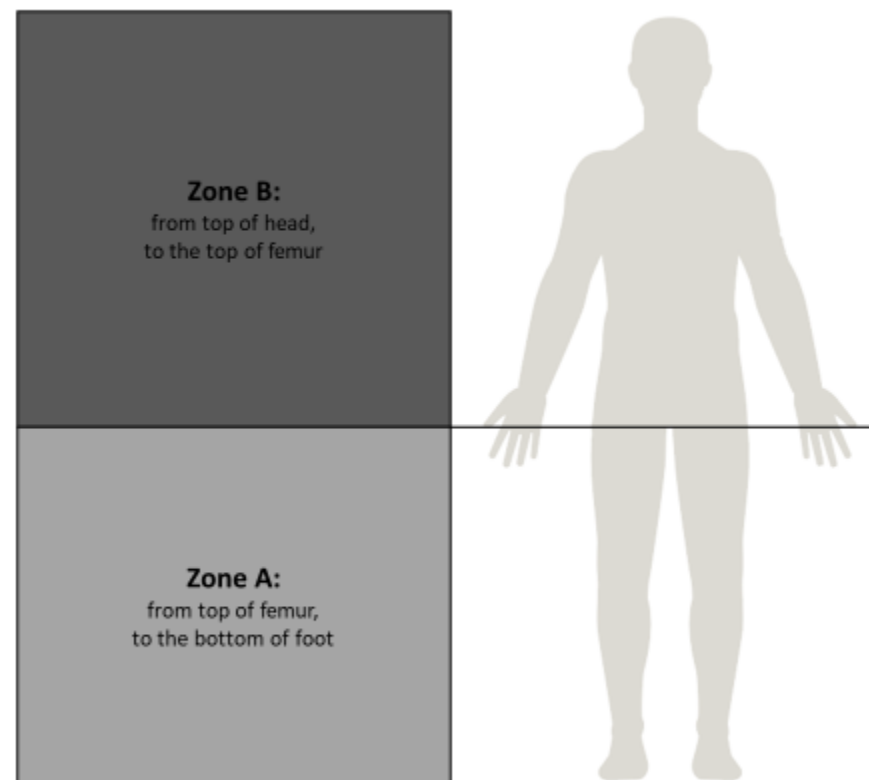


Figure 23



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

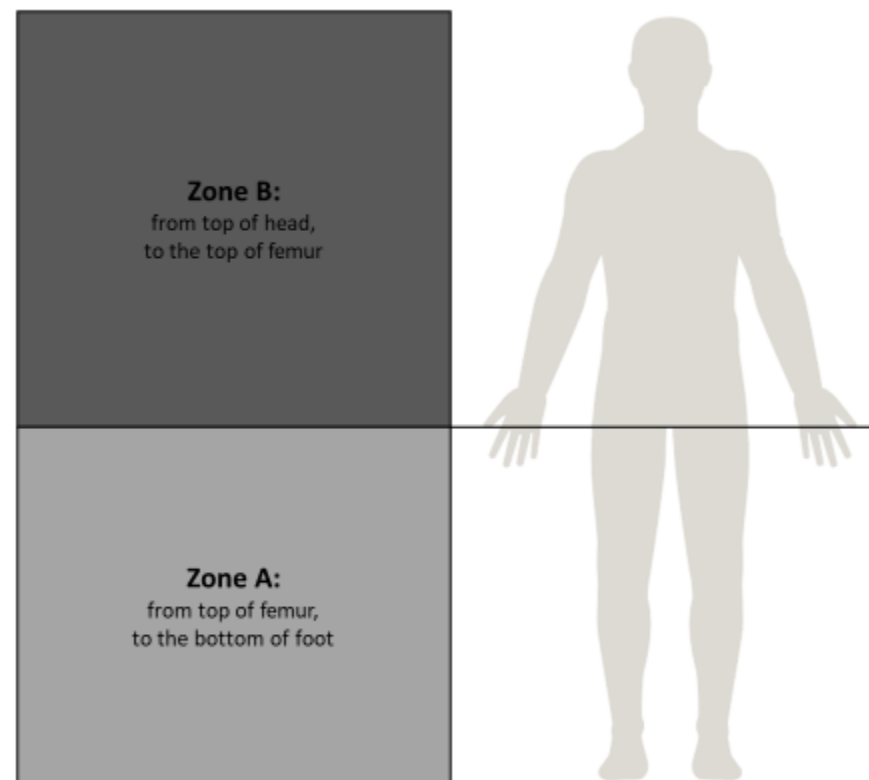


Figure 24



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

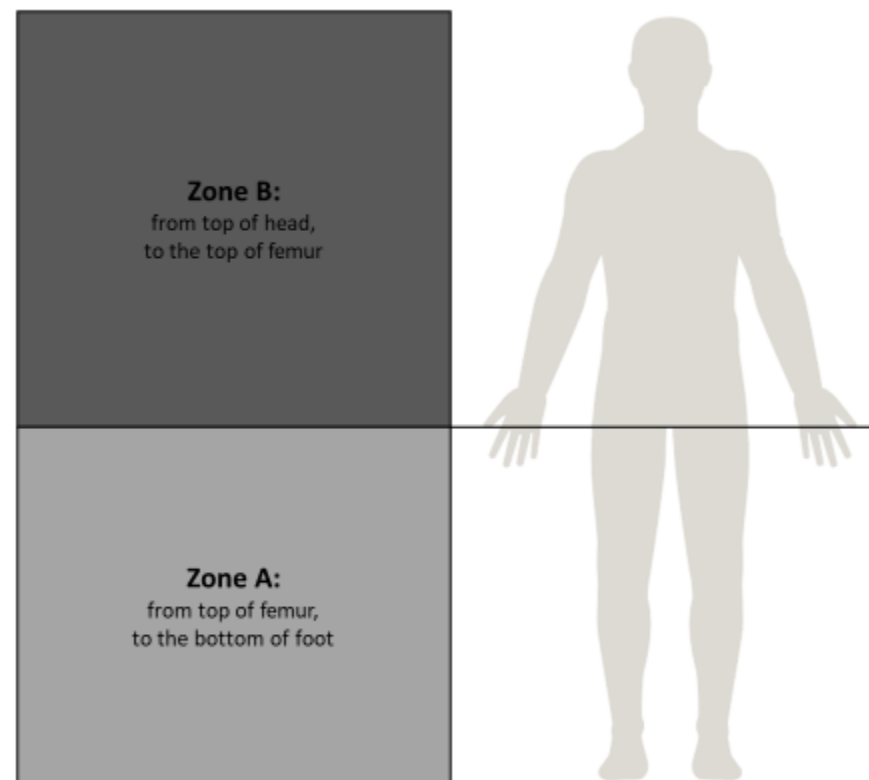


Figure 25

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

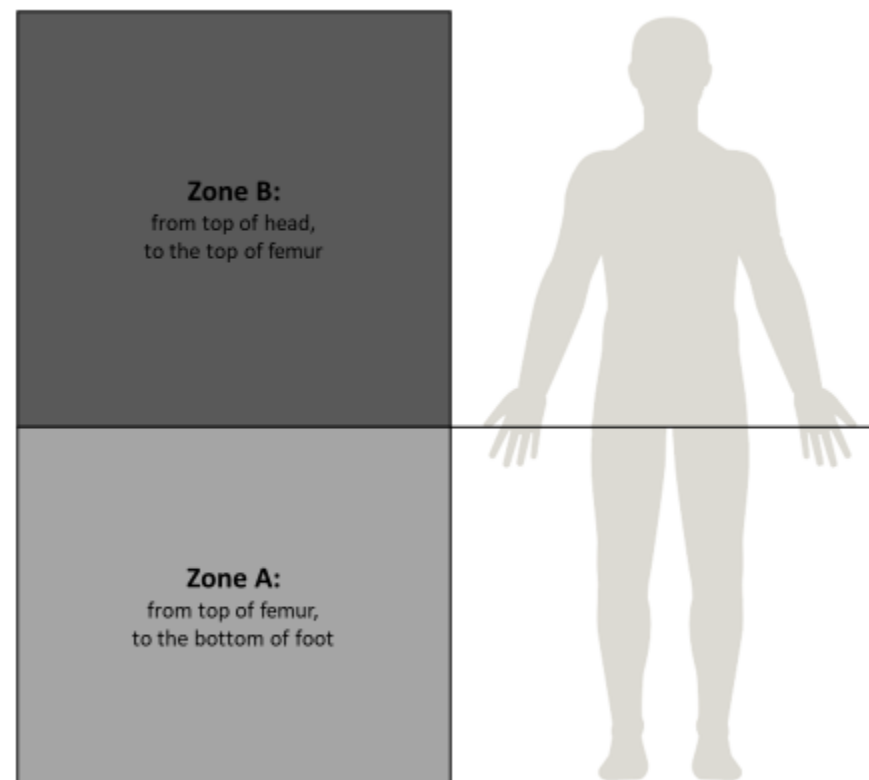


Figure 26

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

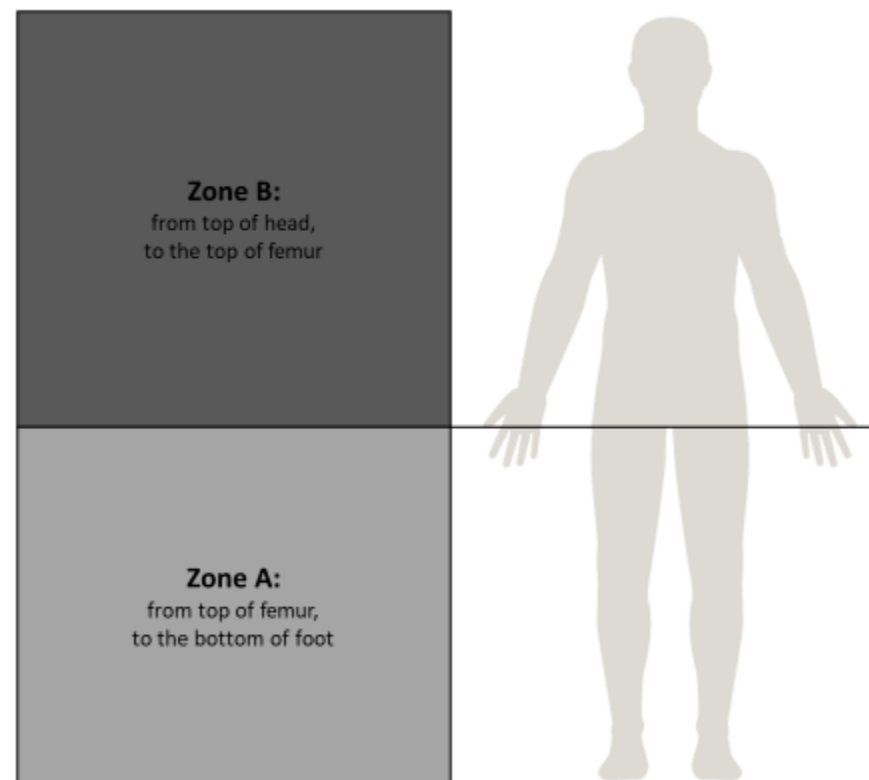


Figure 27

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

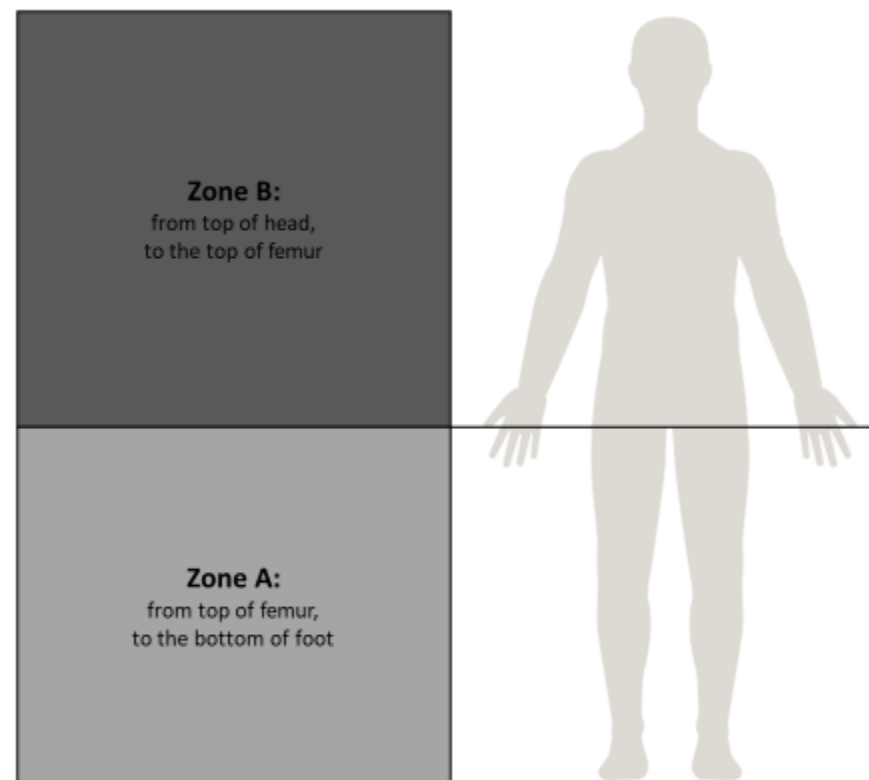


Figure 28

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

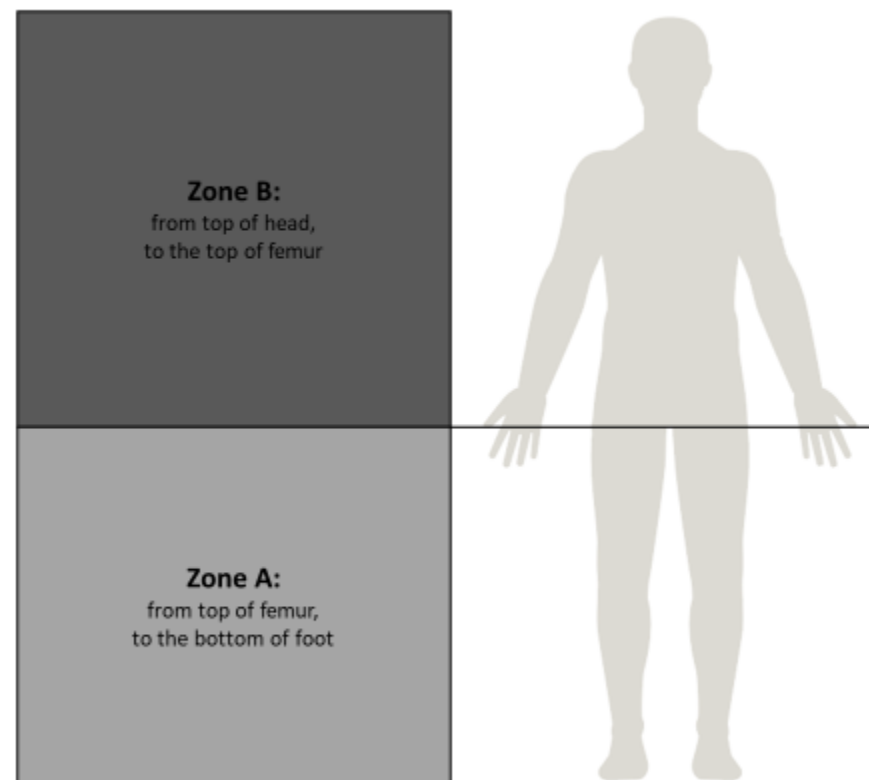


Figure 29

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

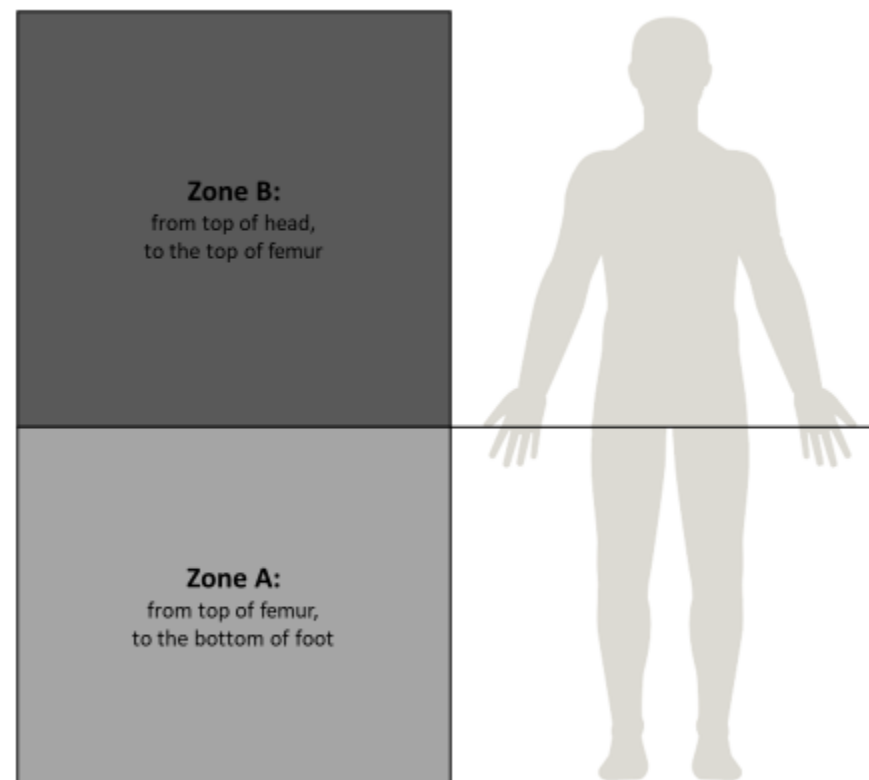



Figure 30

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

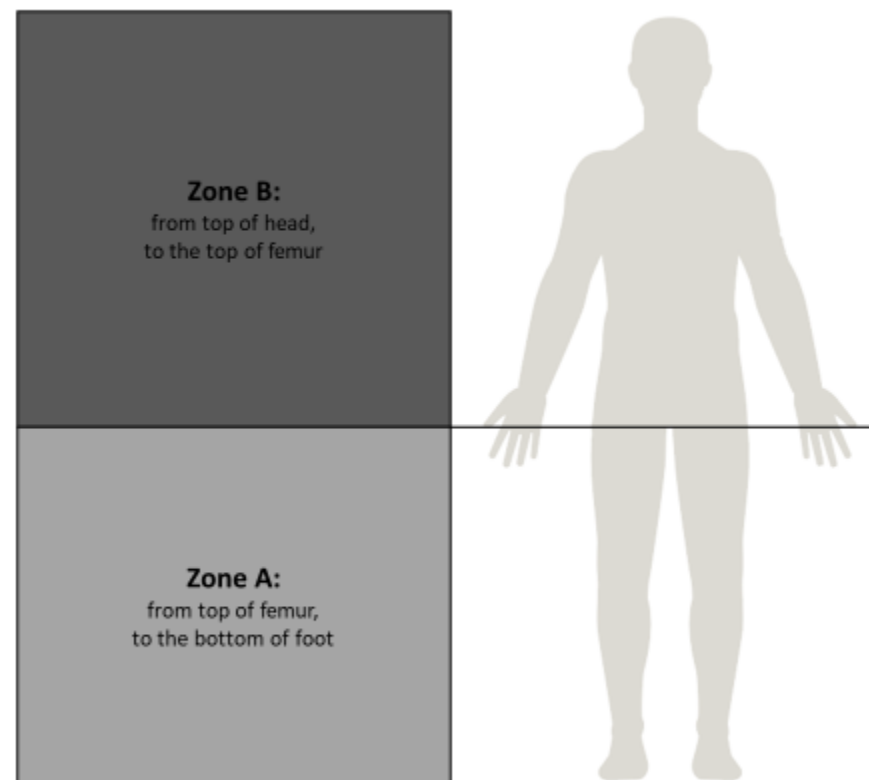**Figure 31**




**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

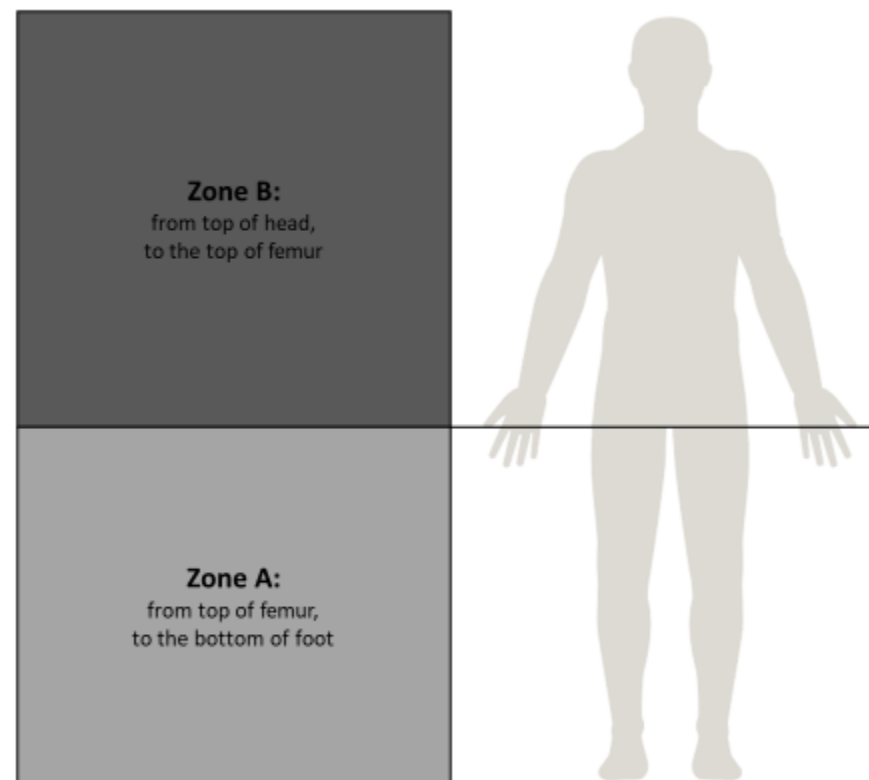**Figure 32**



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

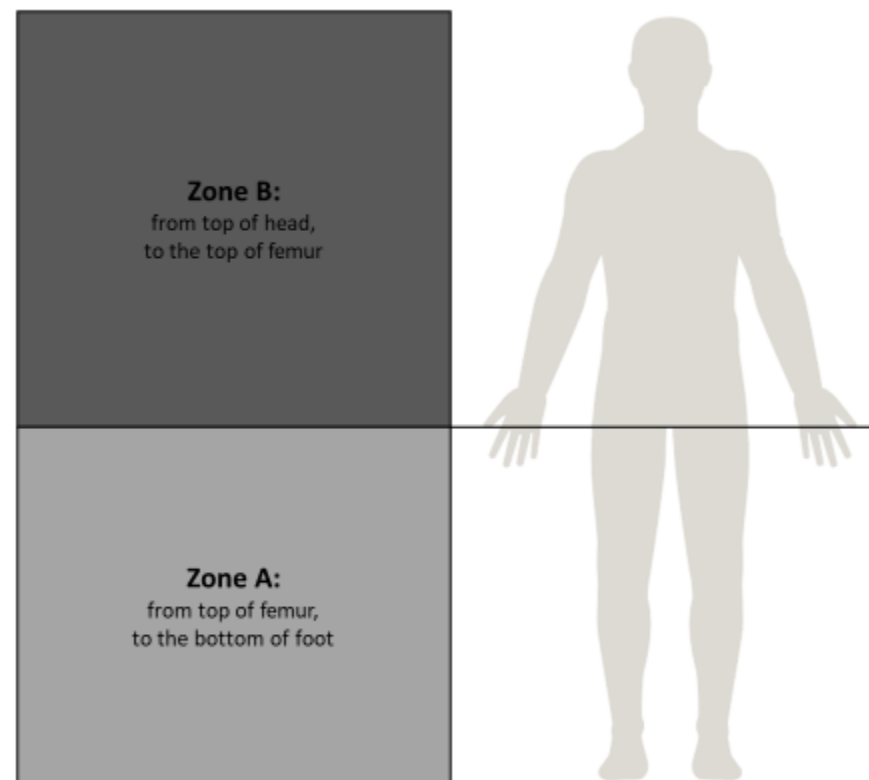


Figure 33

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

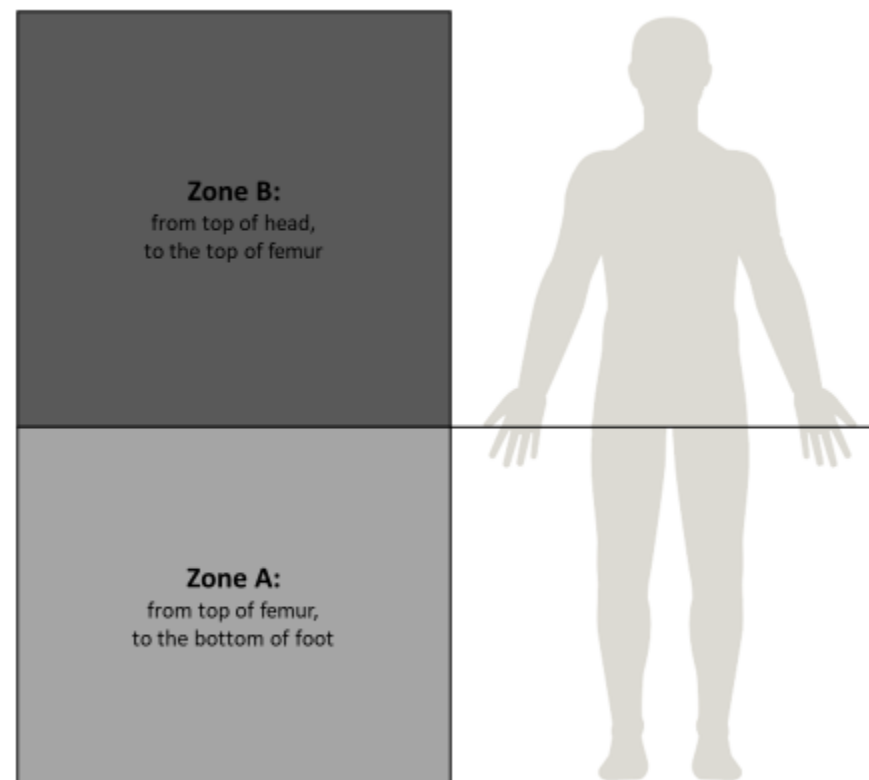


Figure 34

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

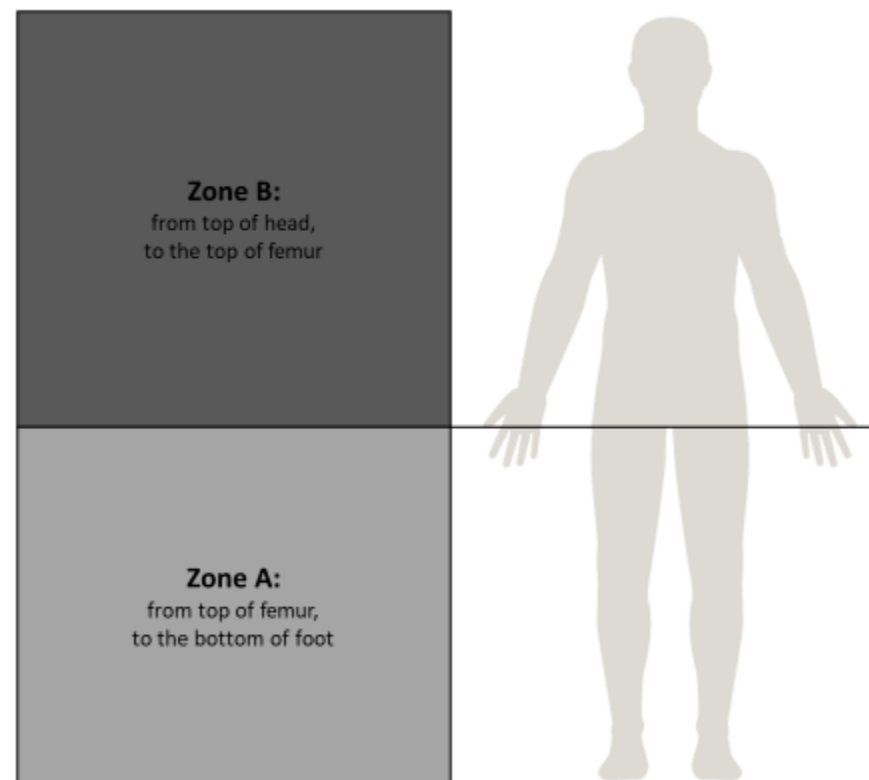


Figure 35

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

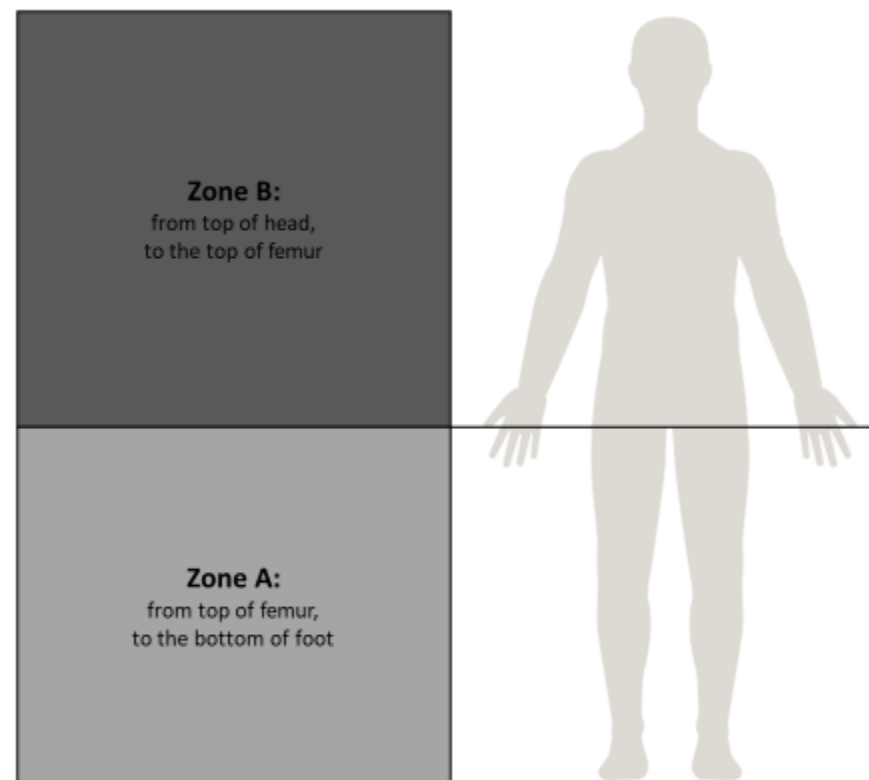


Figure 36

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

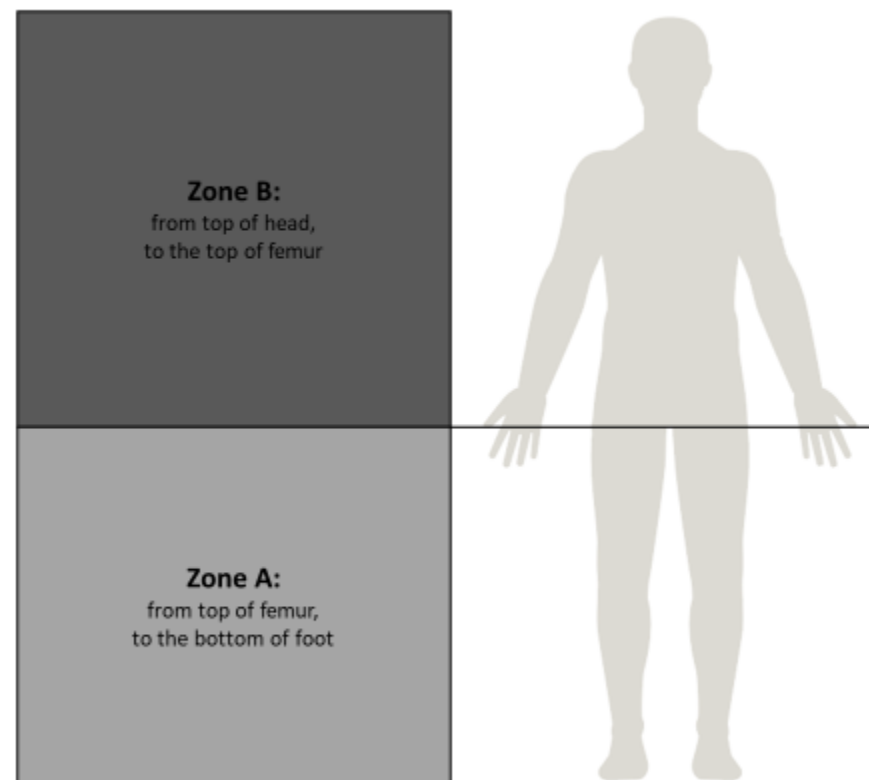


Figure 37

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

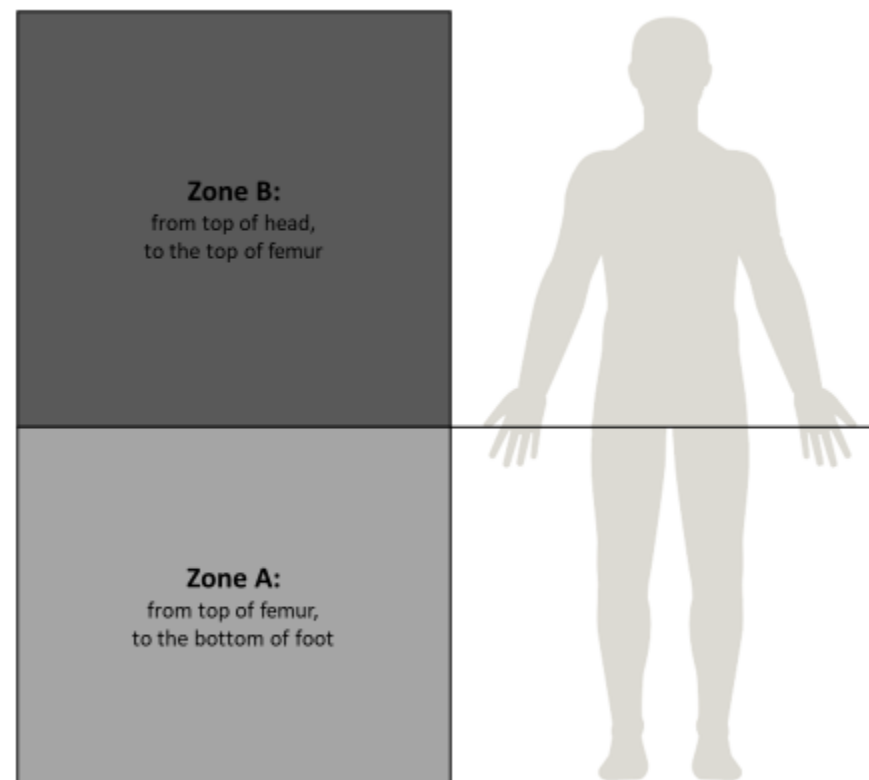


Figure 38

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

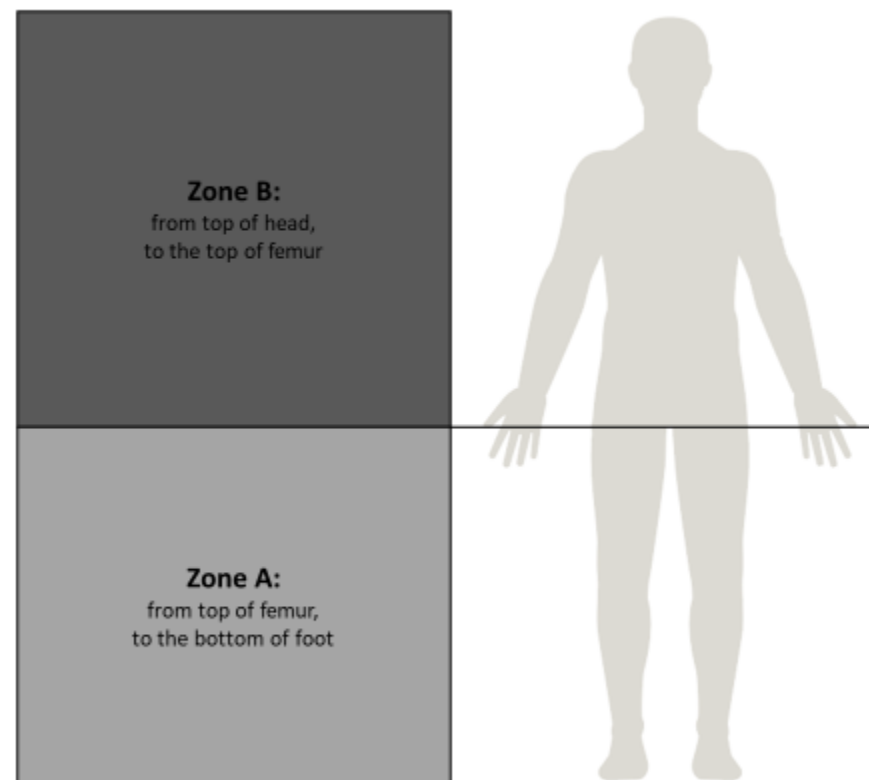


Figure 39



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.0$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

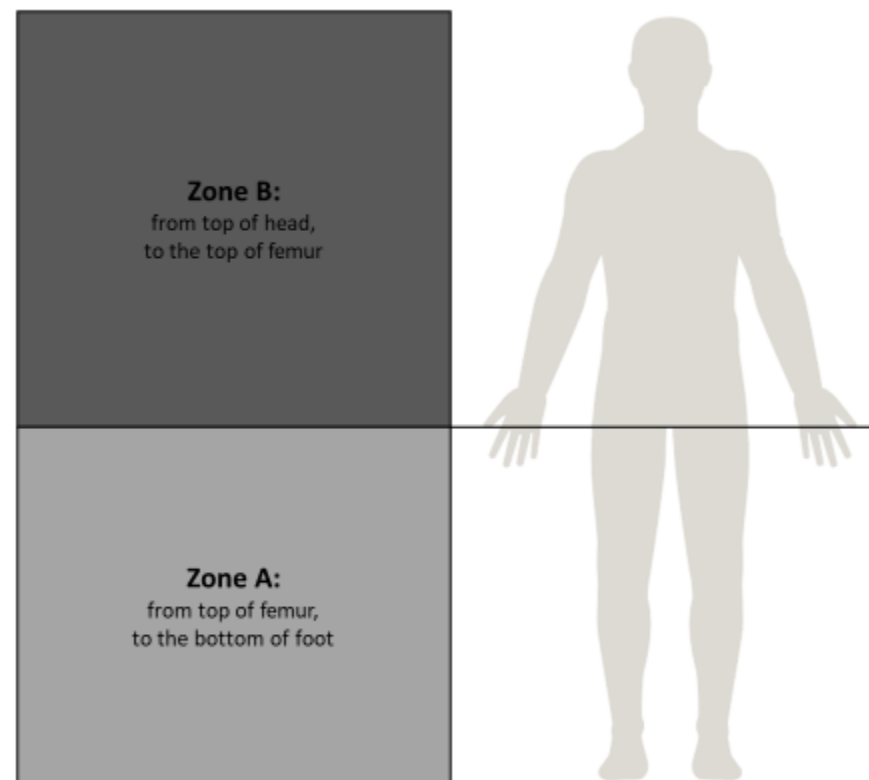


Figure 40



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.0$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

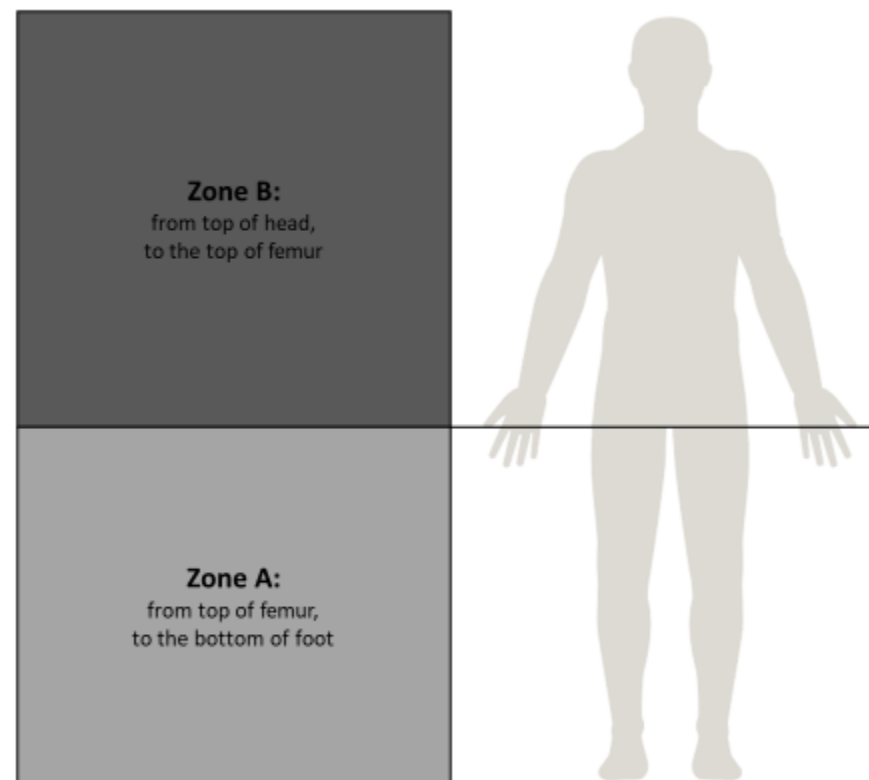


Figure 41

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.1$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

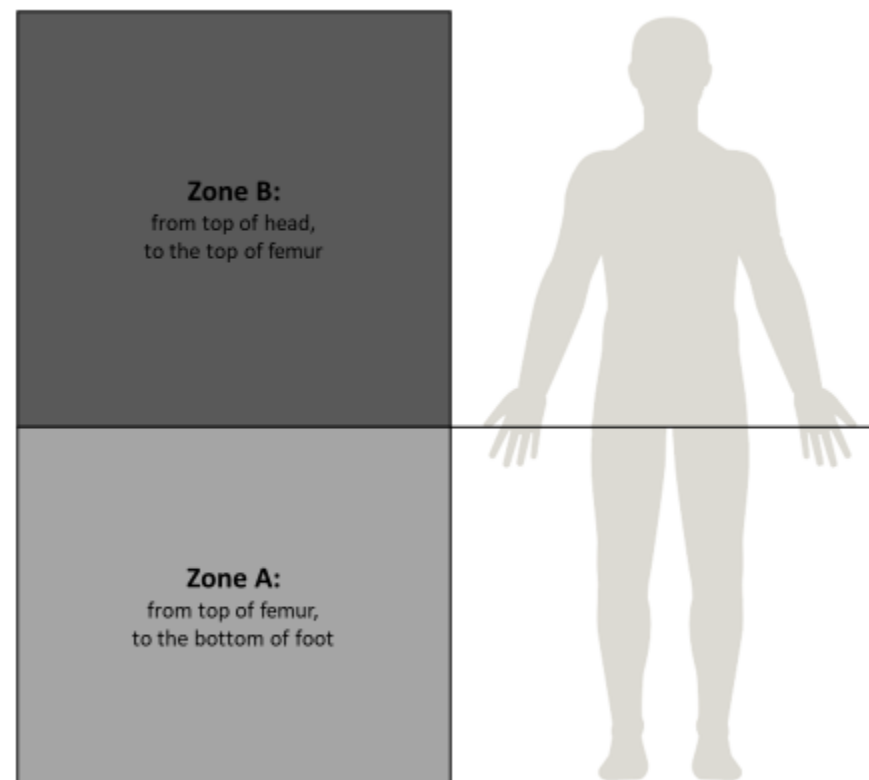


Figure 42

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.2$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

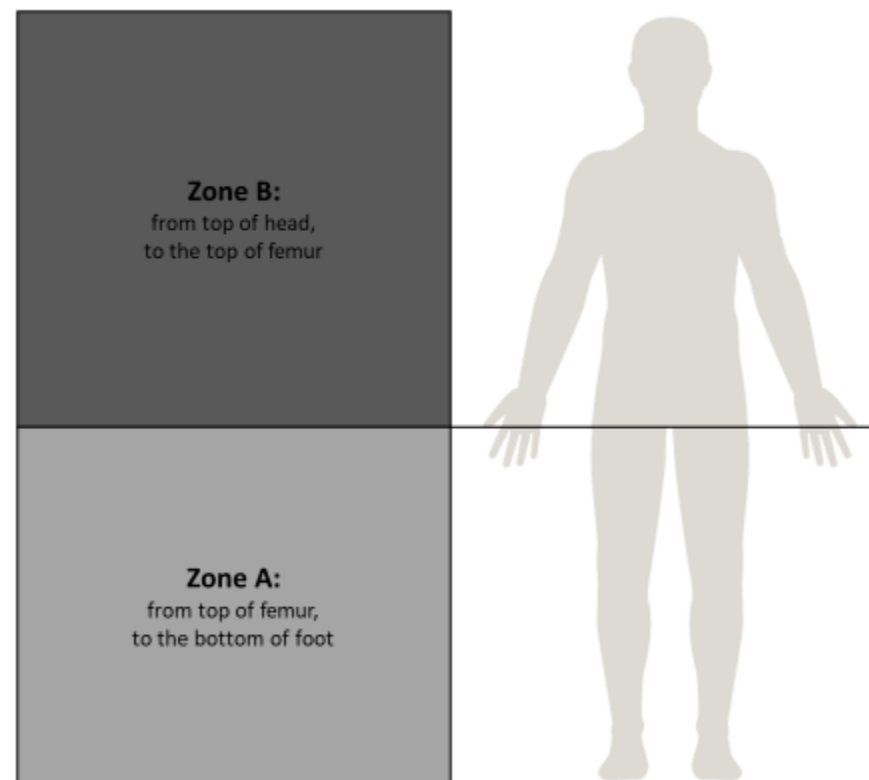


Figure 43

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.2$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

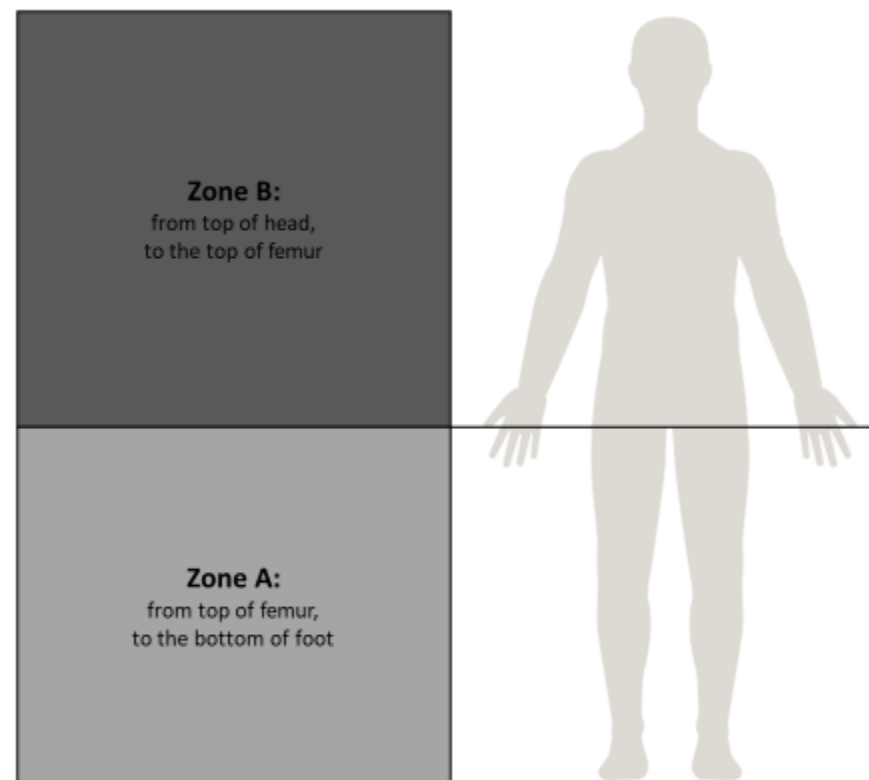


Figure 44

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.2$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

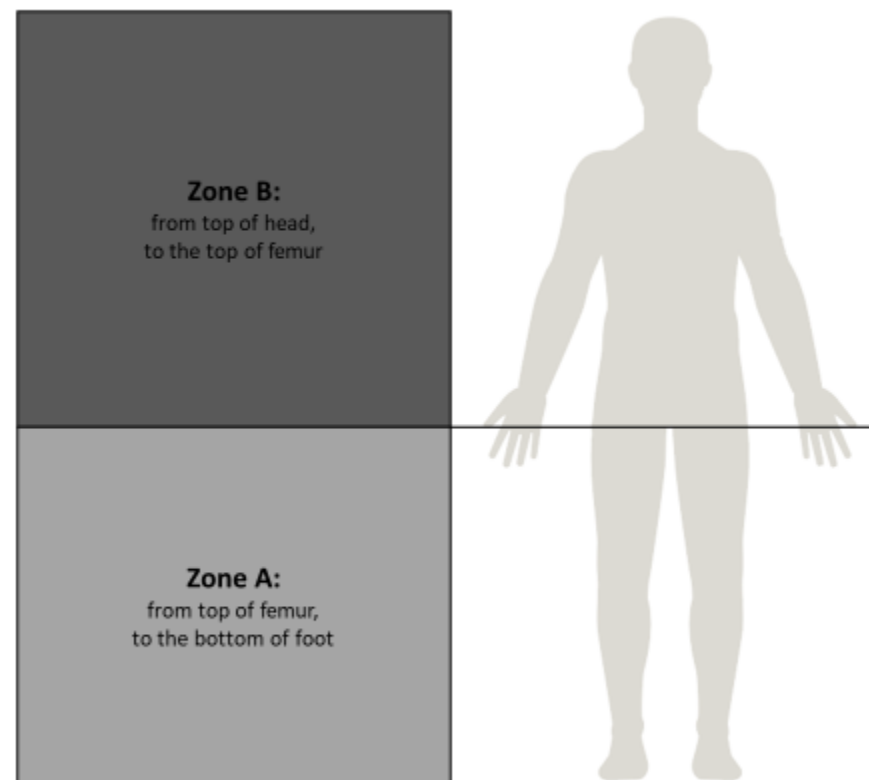


Figure 45

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.4$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

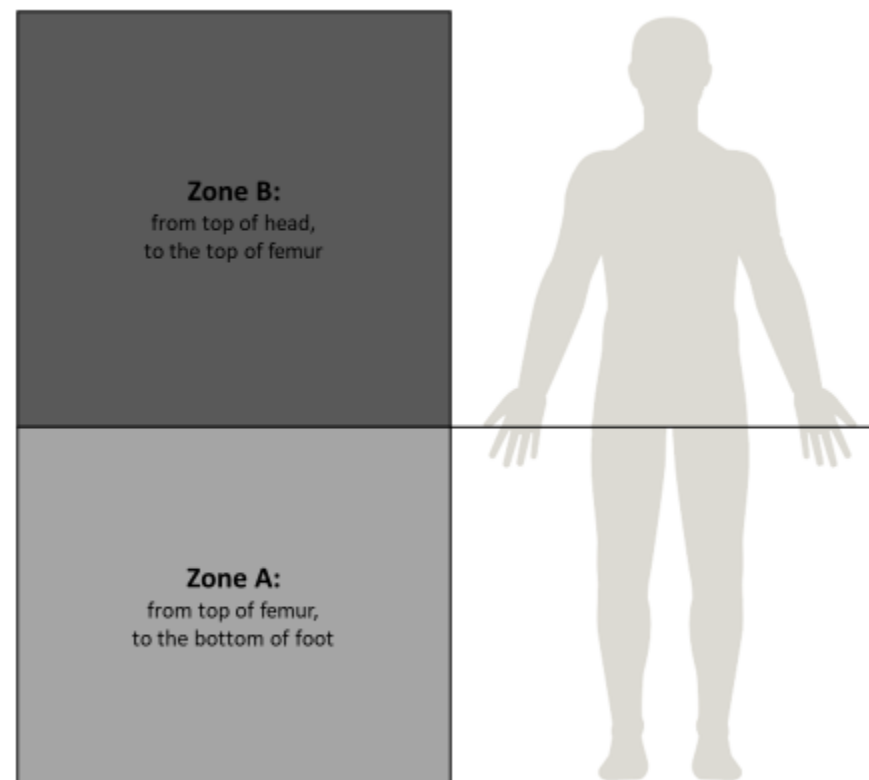


Figure 46

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.5$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

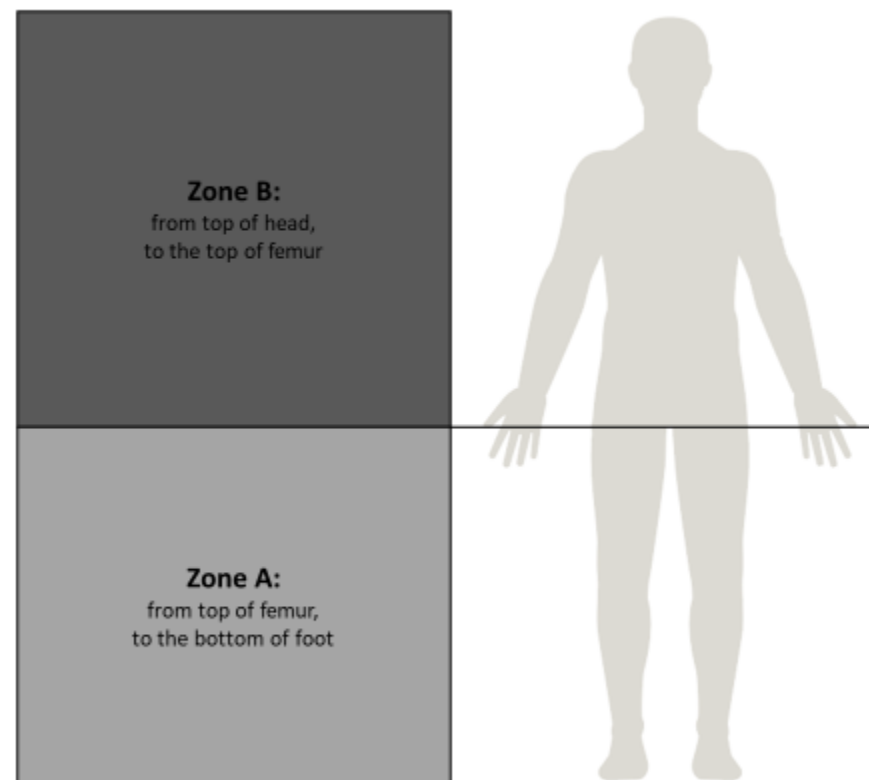


Figure 47



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.5$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

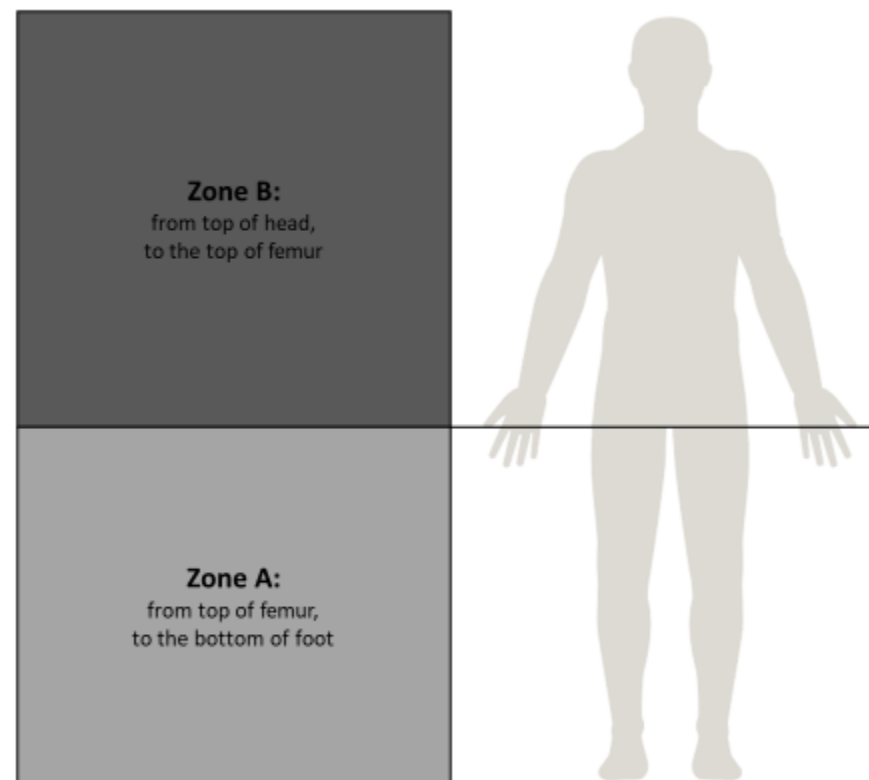


Figure 48



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.8$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

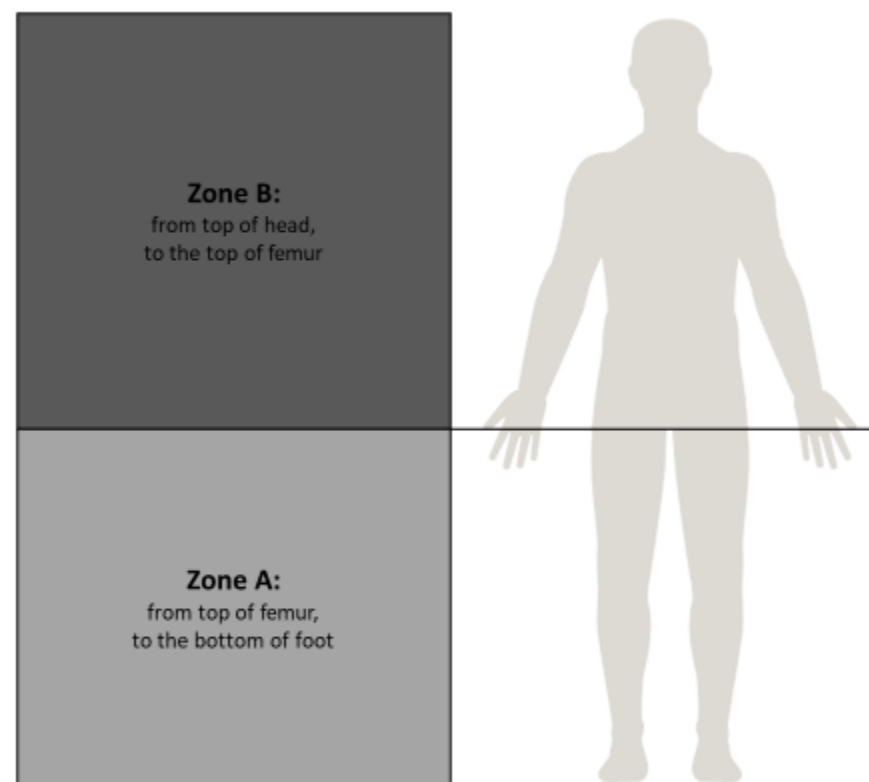


Figure 49

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.8$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

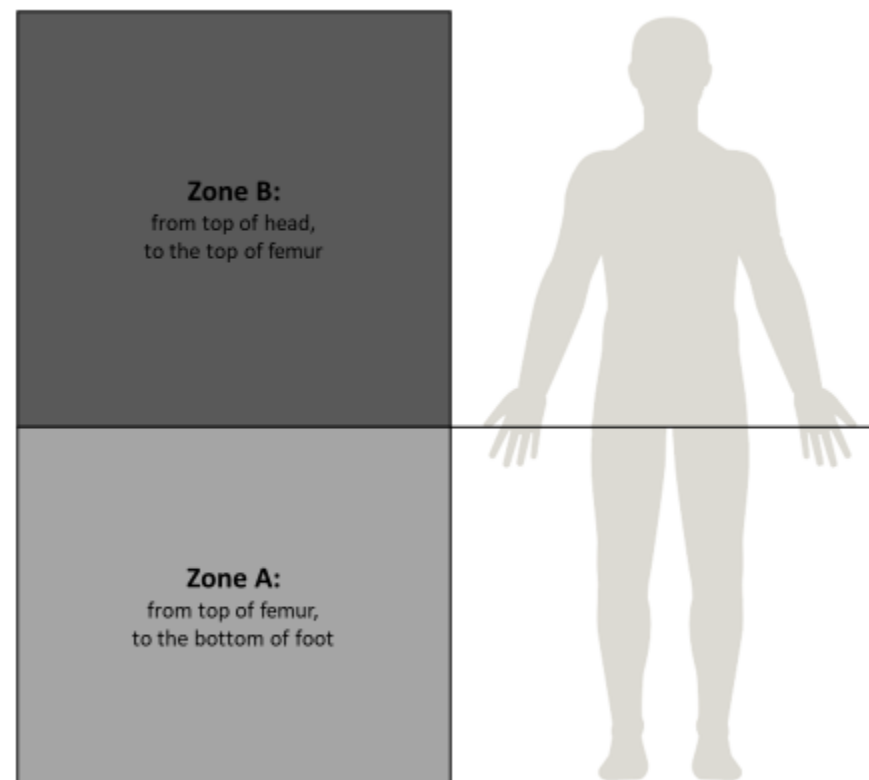


Figure 50

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.9$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

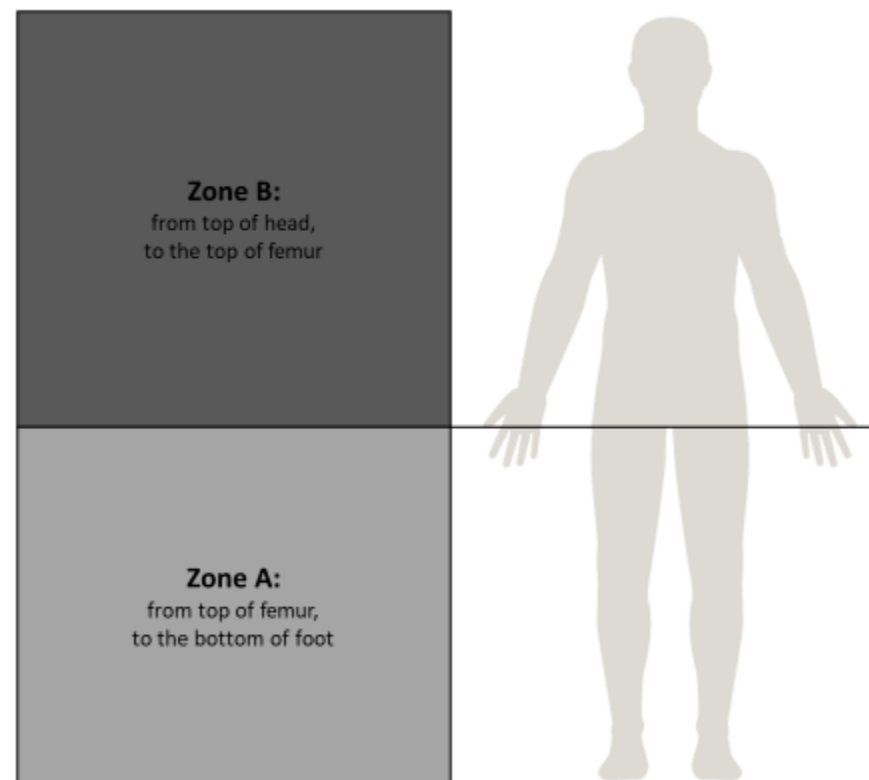


Figure 51

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

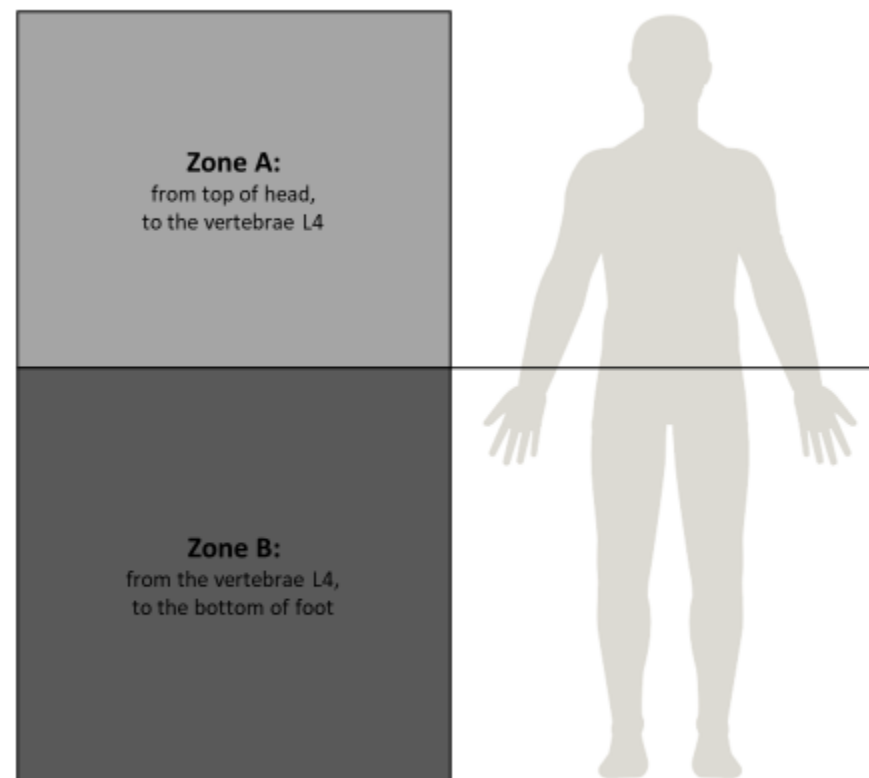


Figure 52

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

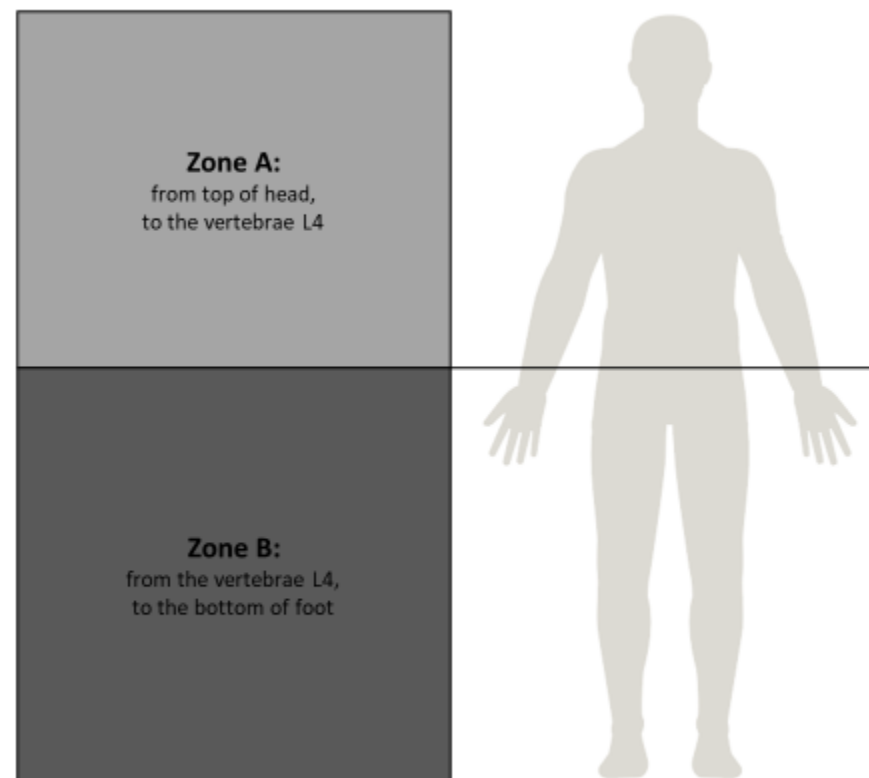


Figure 53

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

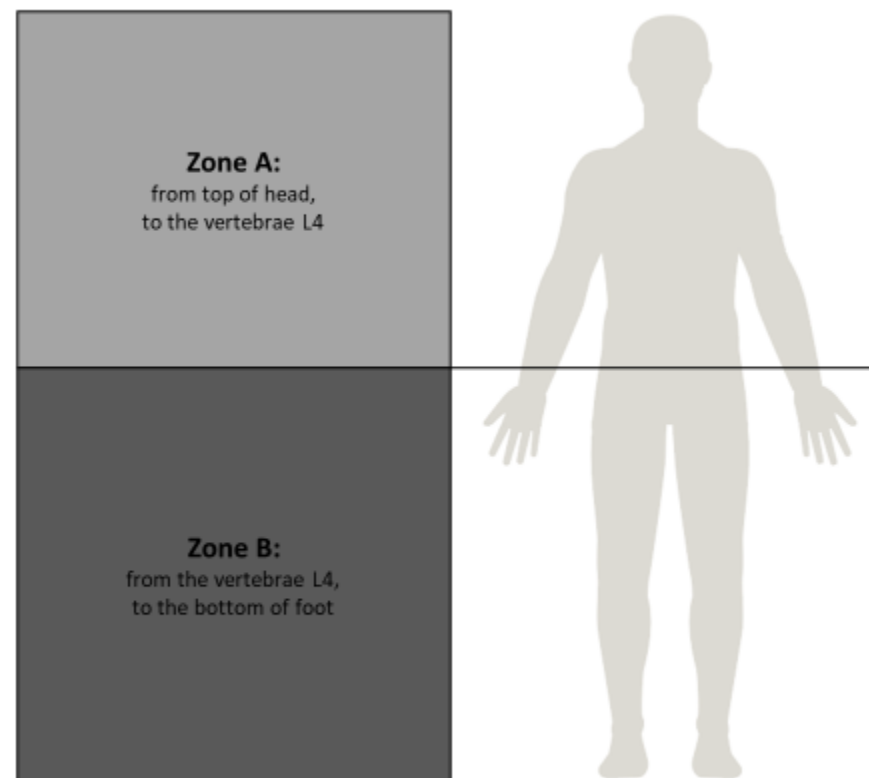


Figure 54

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

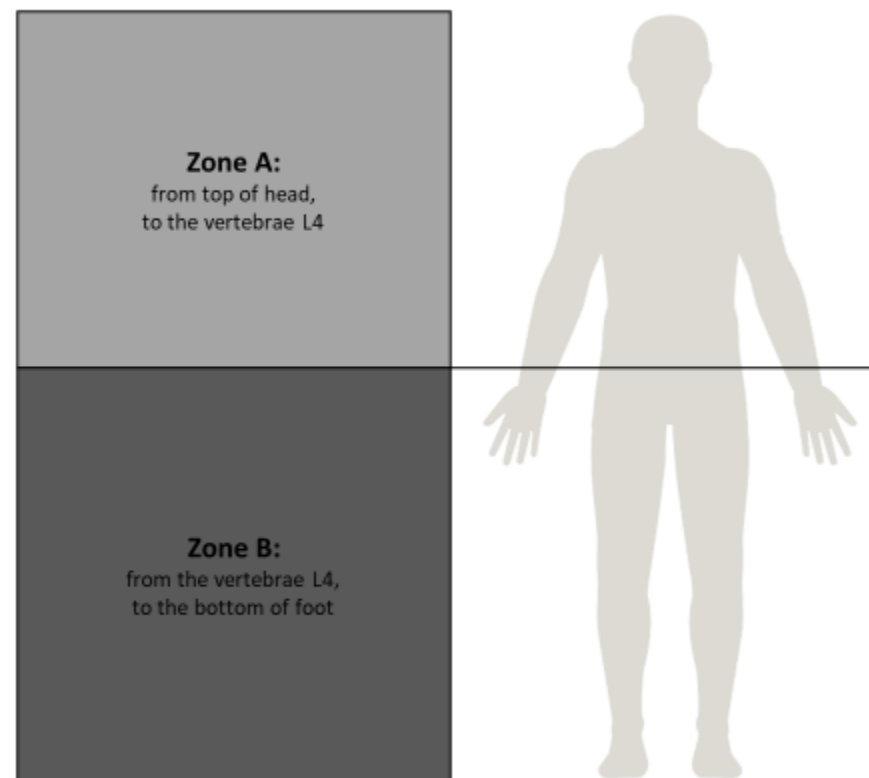


Figure 55



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

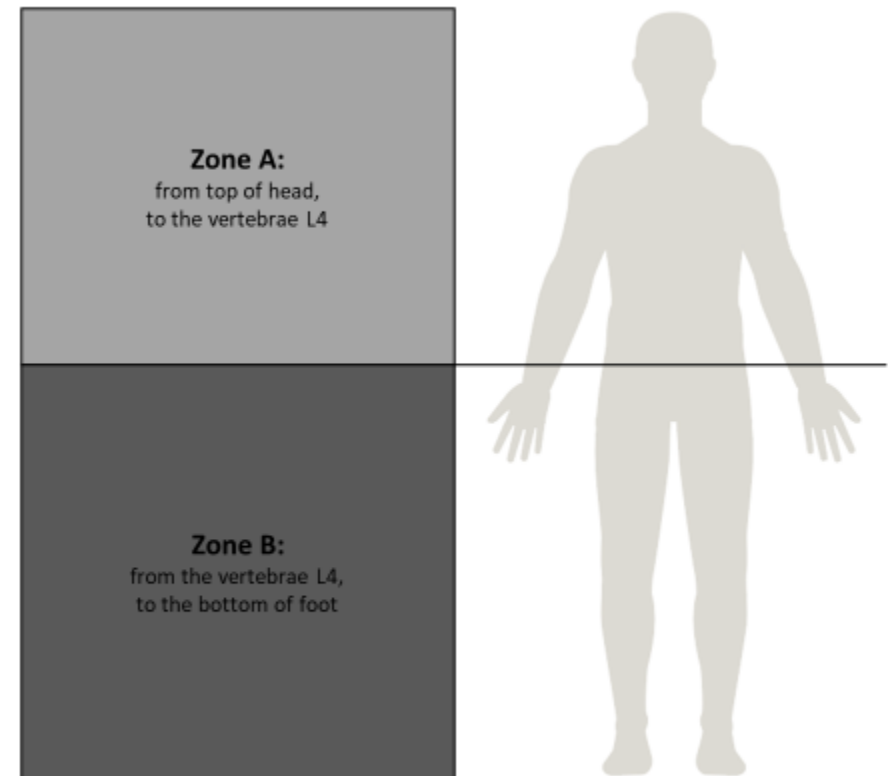


Figure 56



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

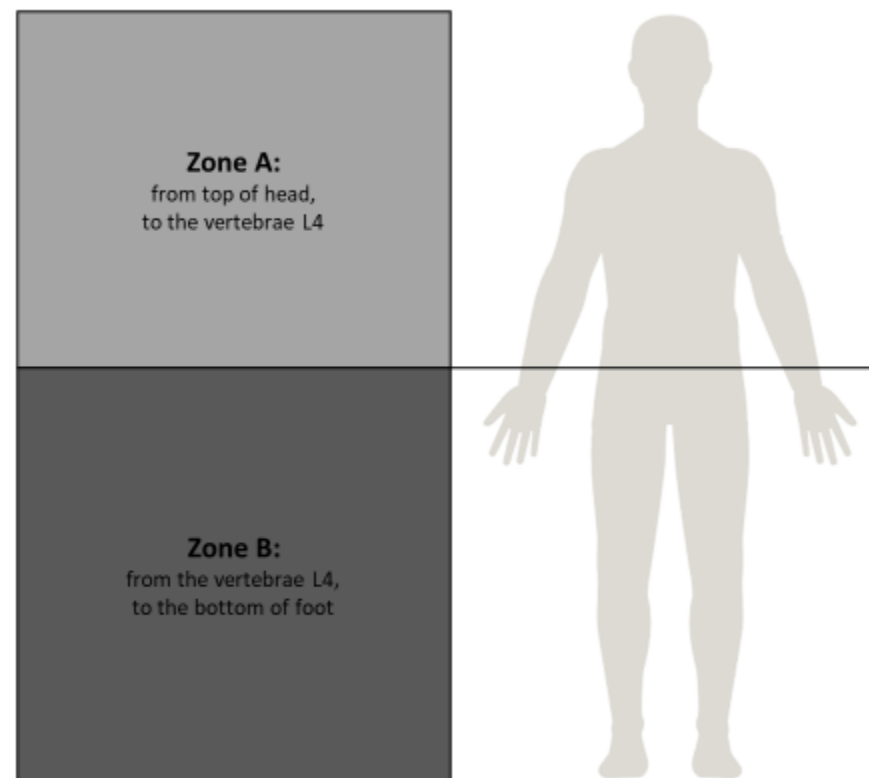


Figure 57

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

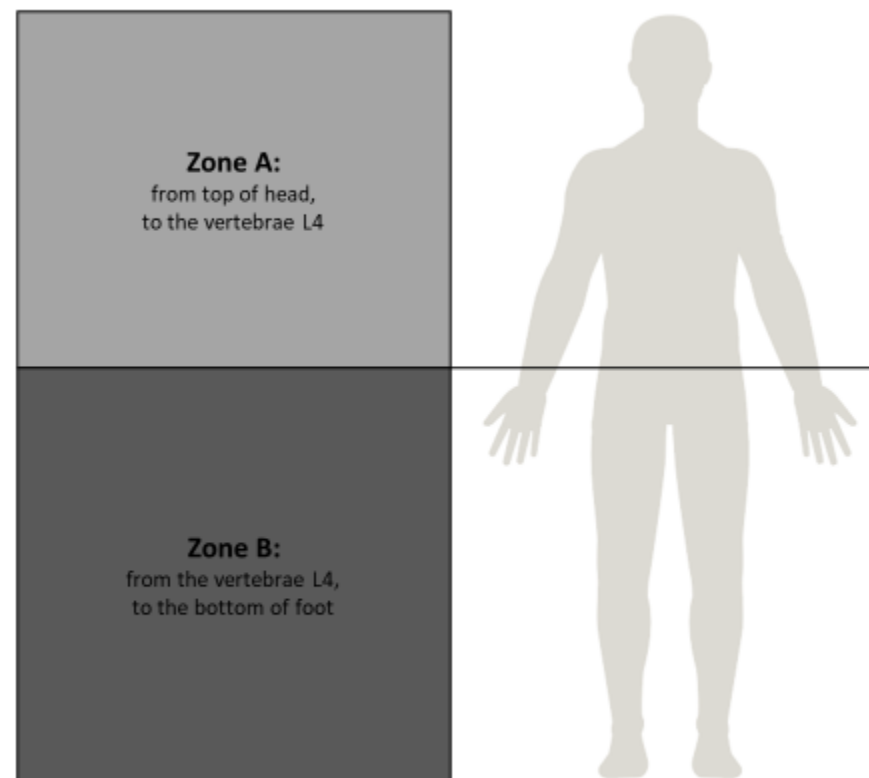


Figure 58

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

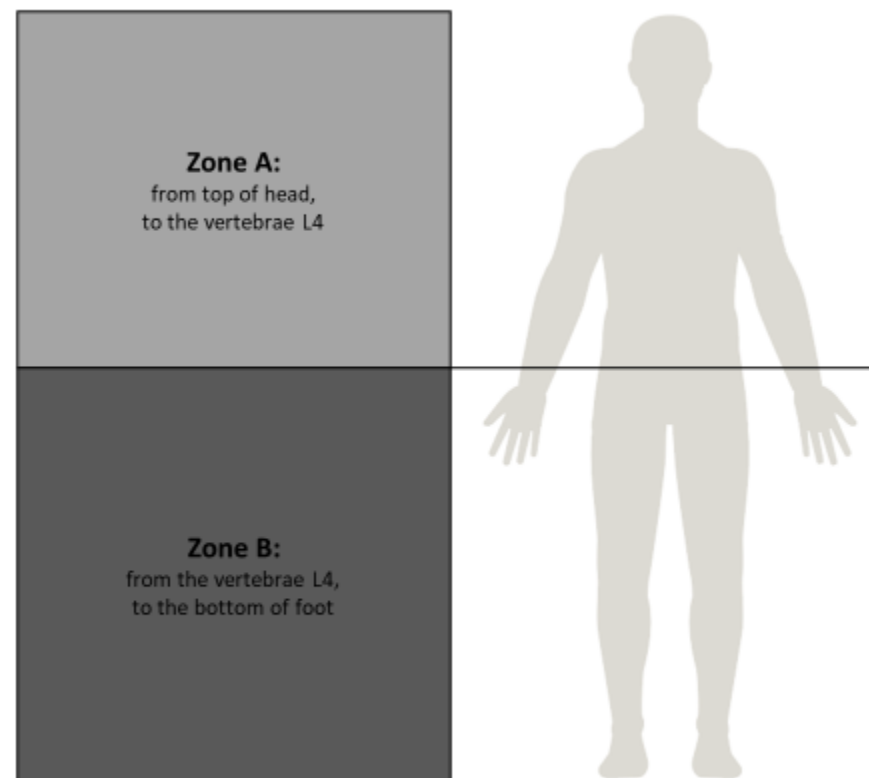


Figure 59

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

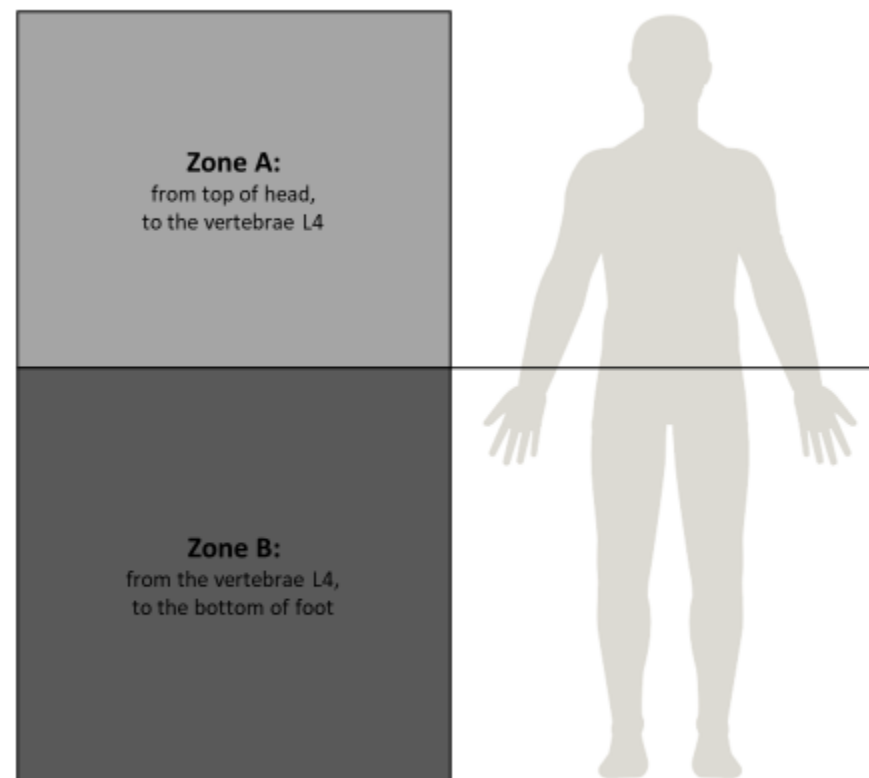


Figure 60

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

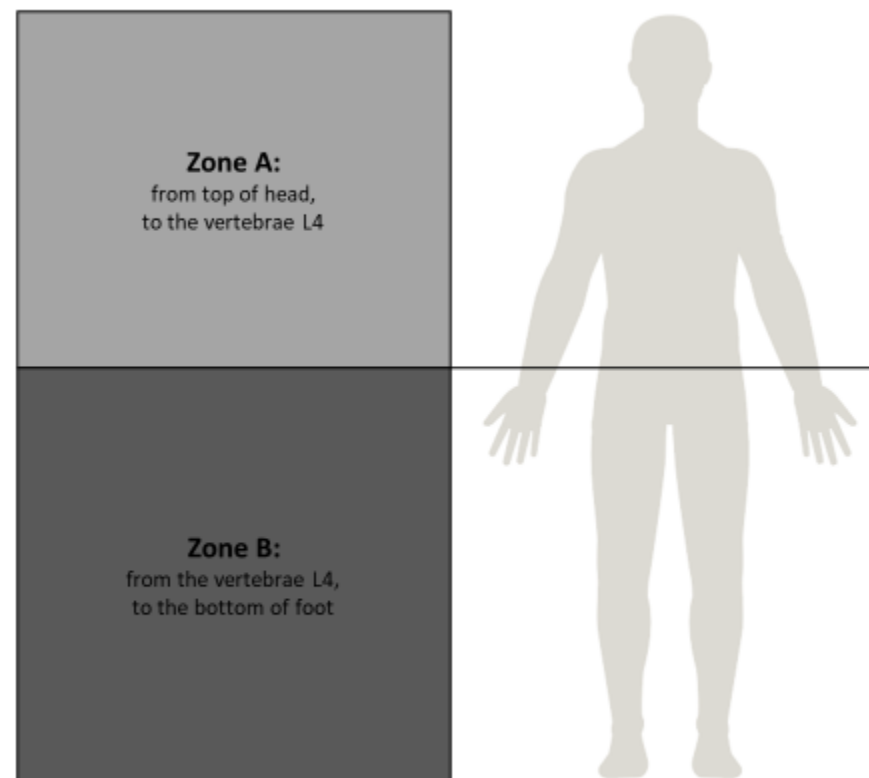


Figure 61

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

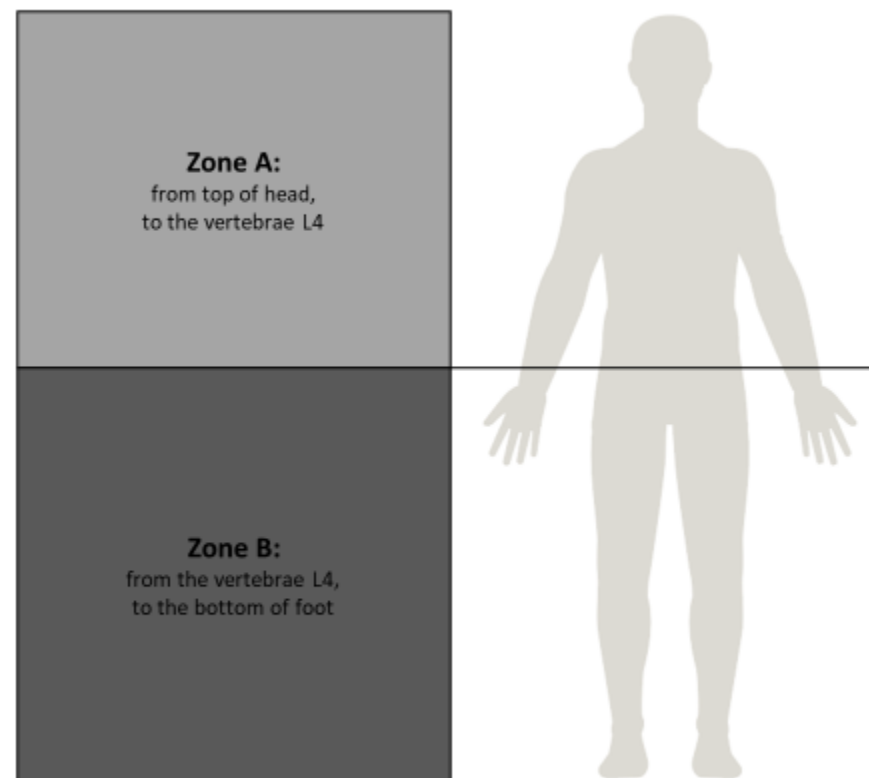


Figure 62

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

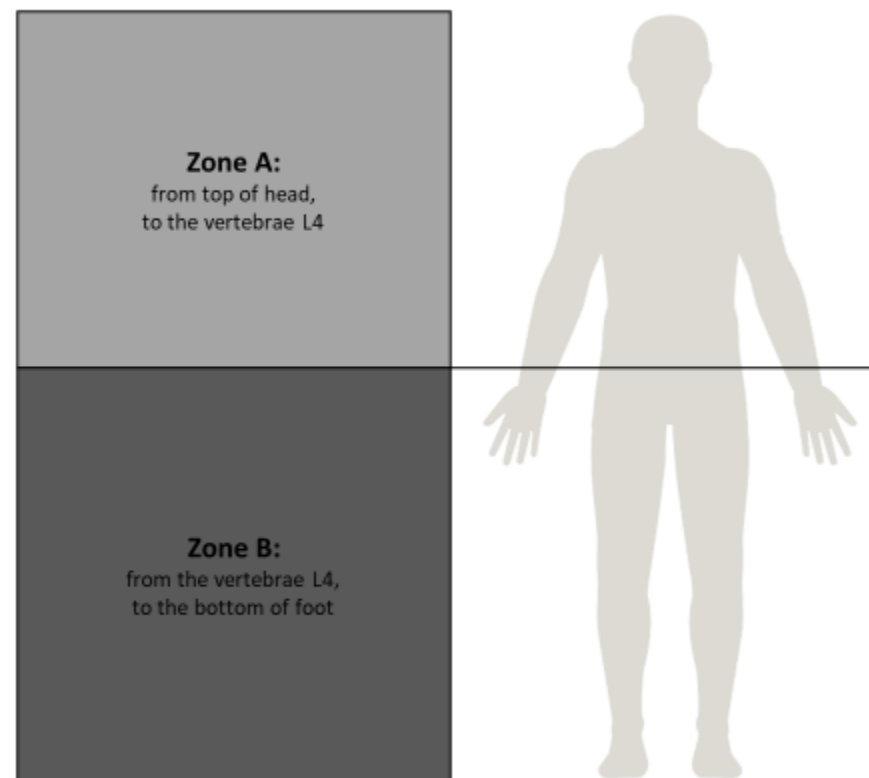


Figure 63



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

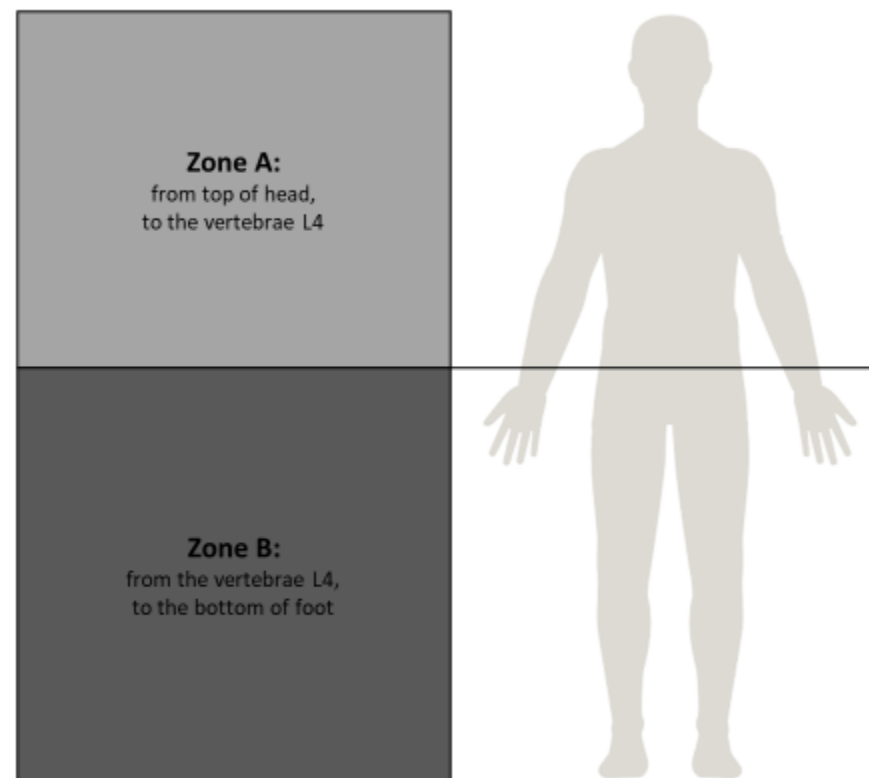


Figure 64



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

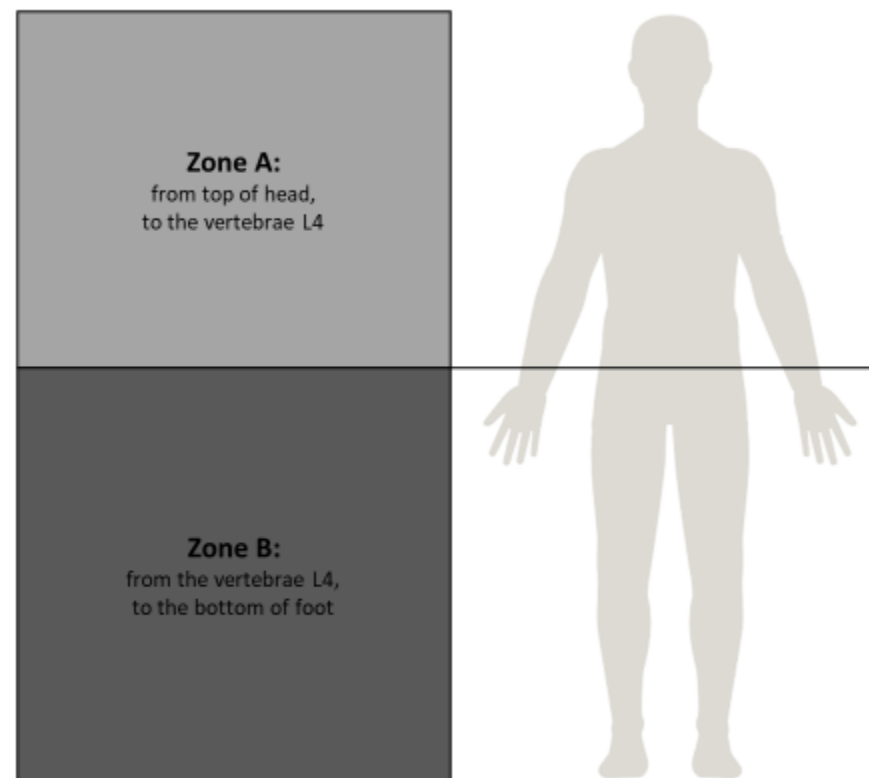


Figure 65

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

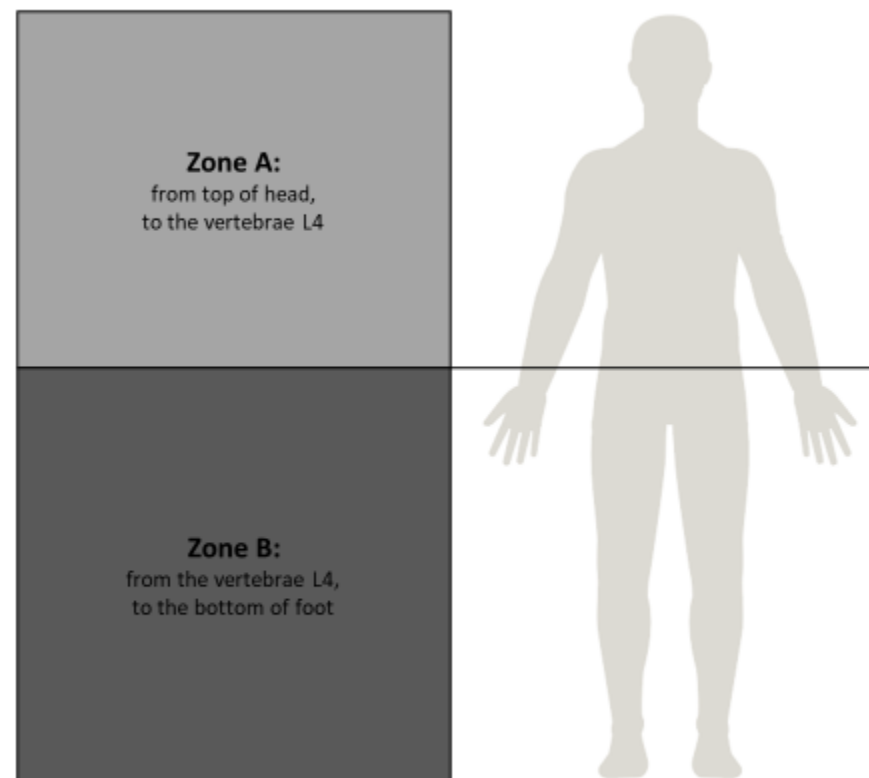


Figure 66

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

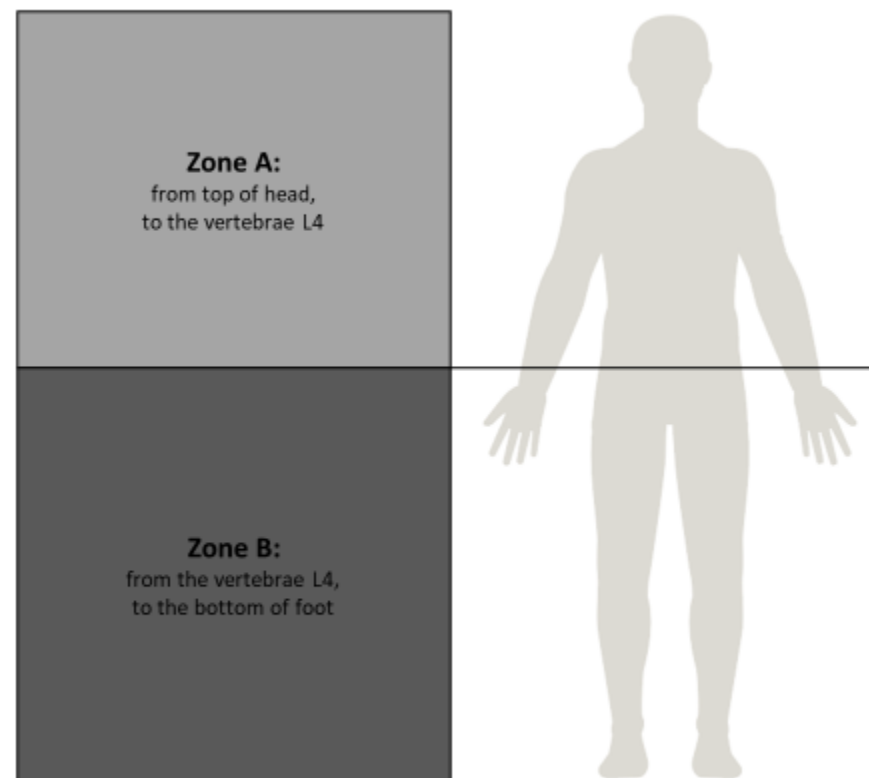


Figure 67

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

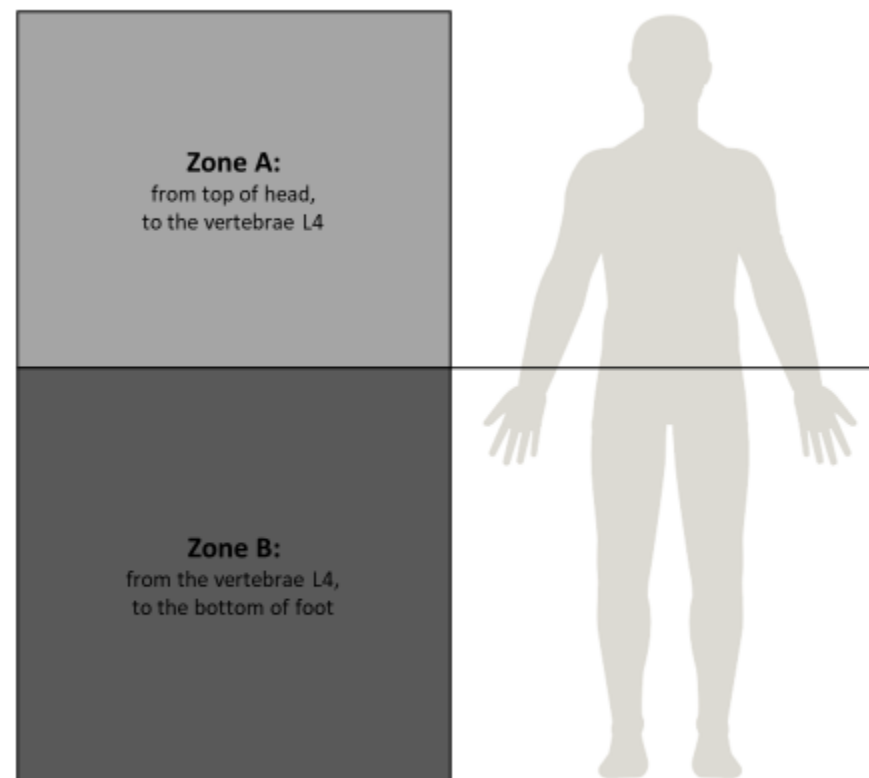


Figure 68

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

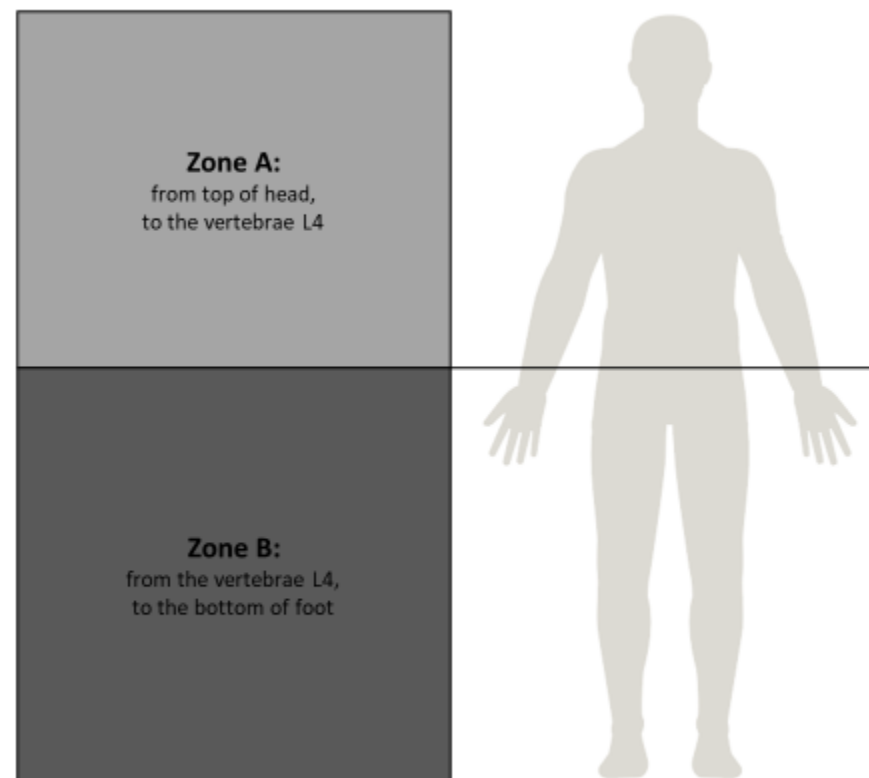


Figure 69

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

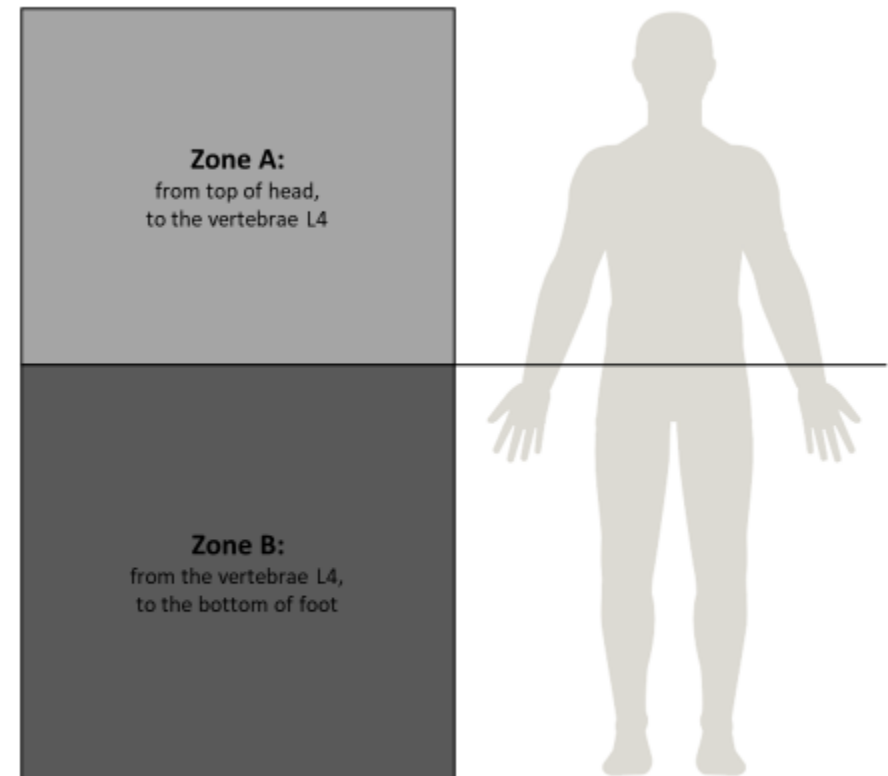


Figure 70

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

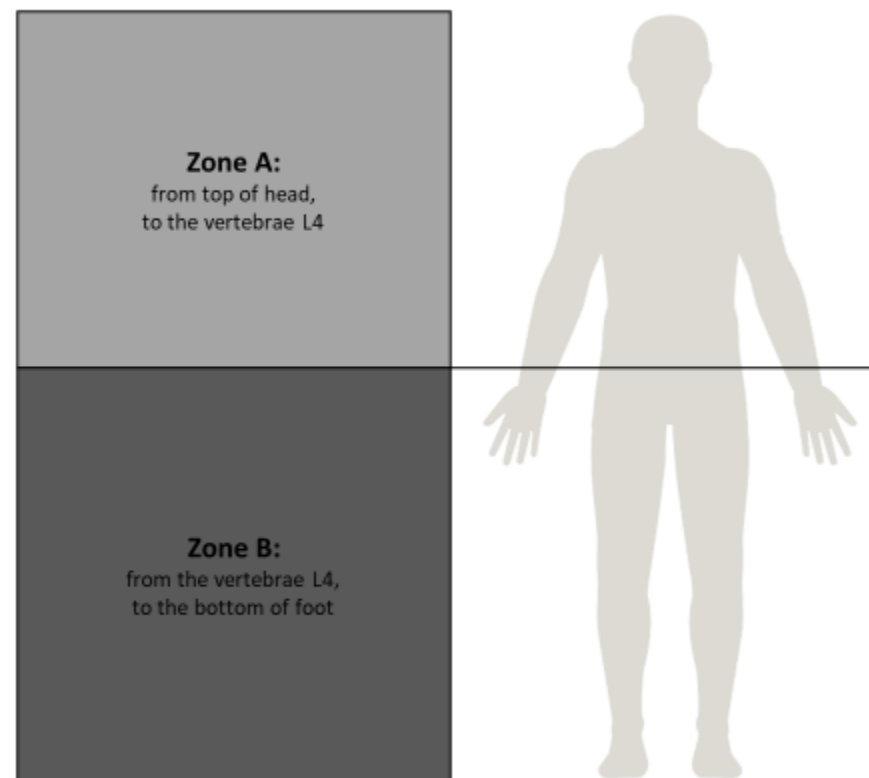


Figure 71



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

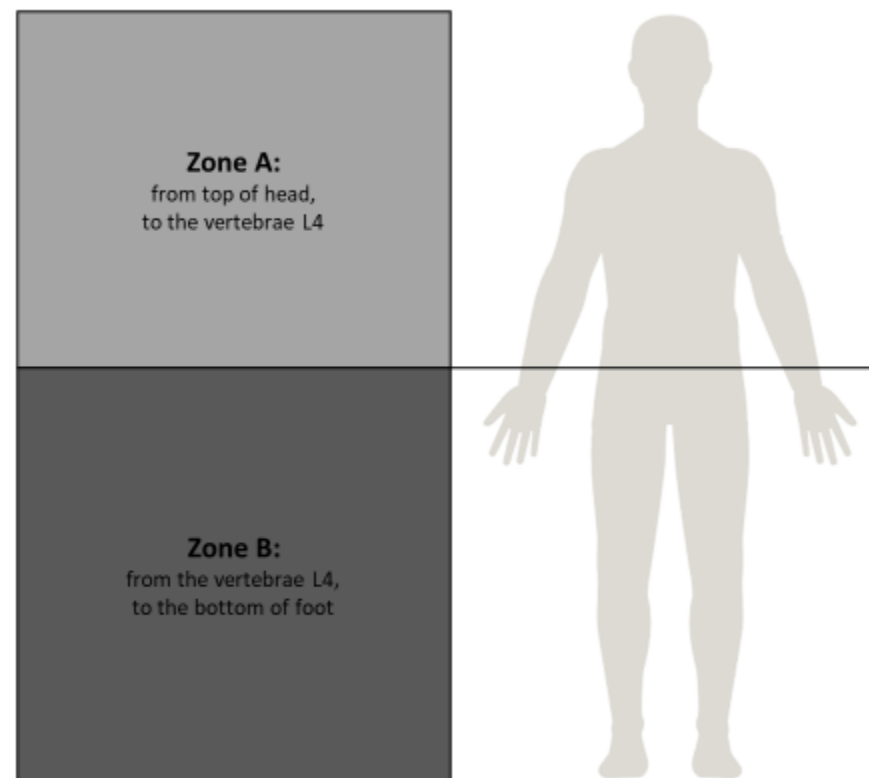


Figure 72



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

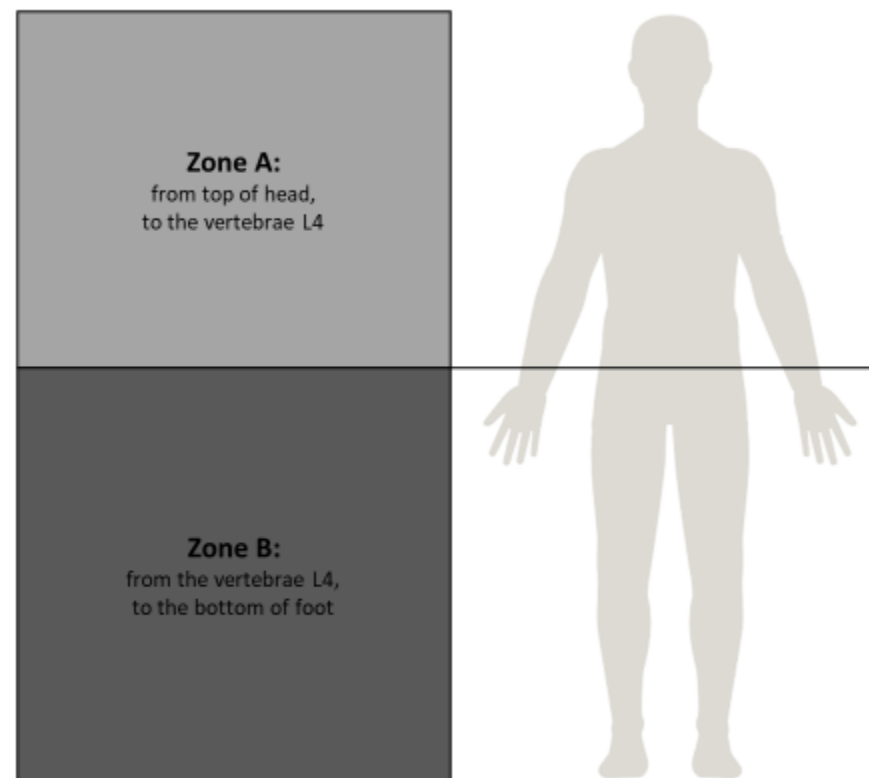


Figure 73

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

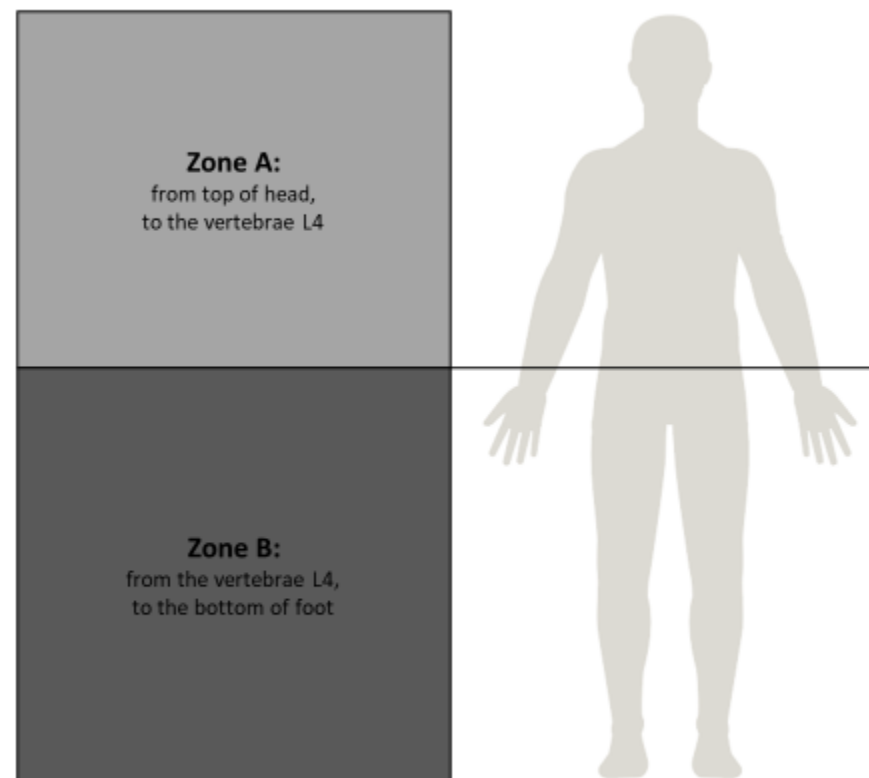


Figure 74

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

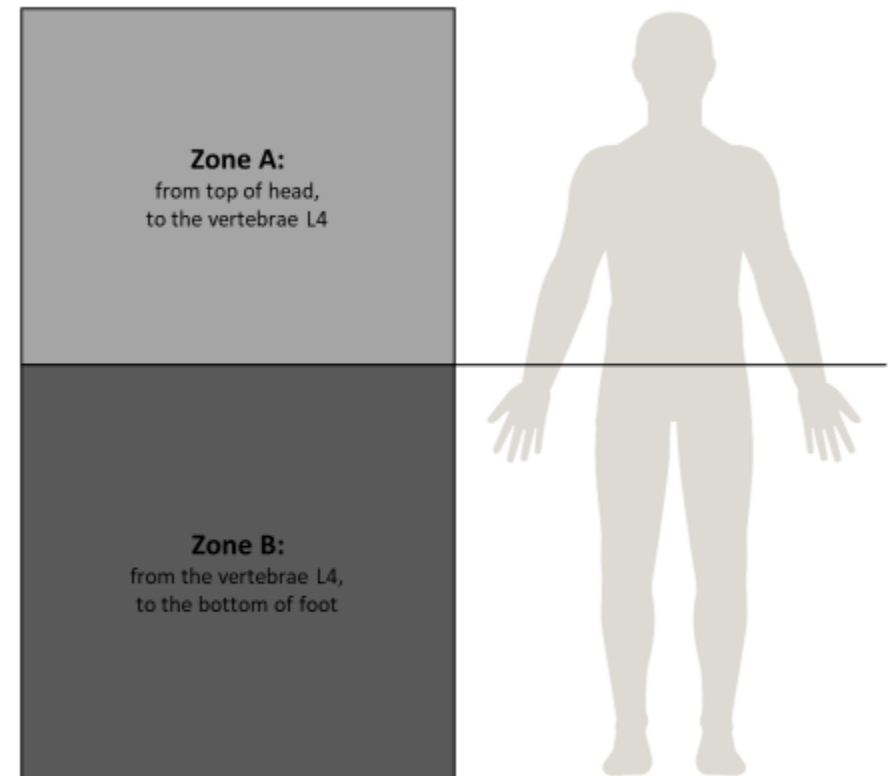


Figure 75

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

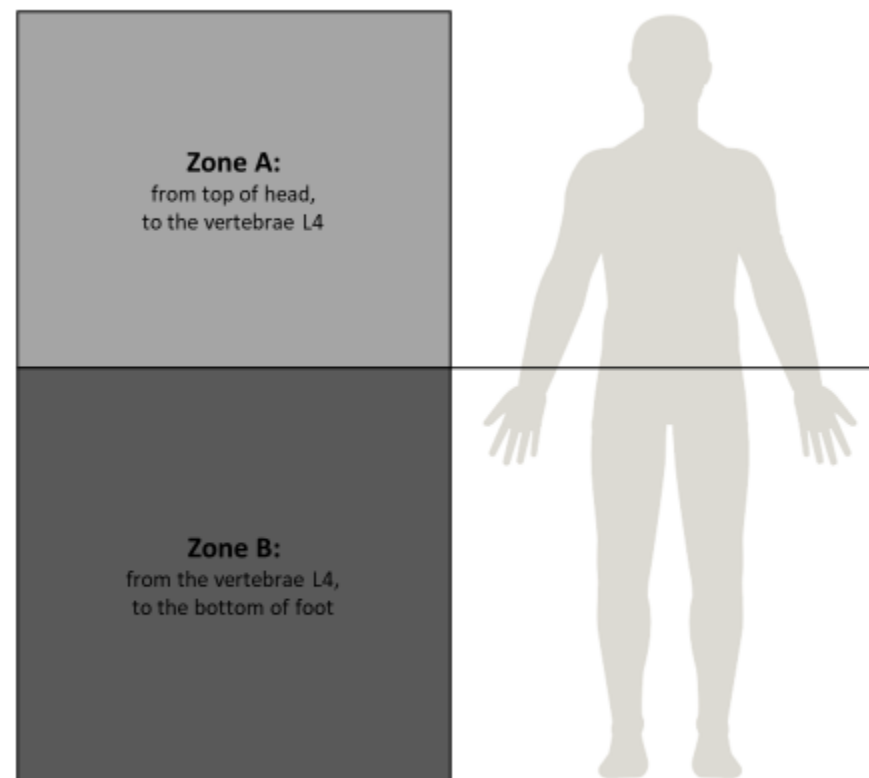


Figure 76

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

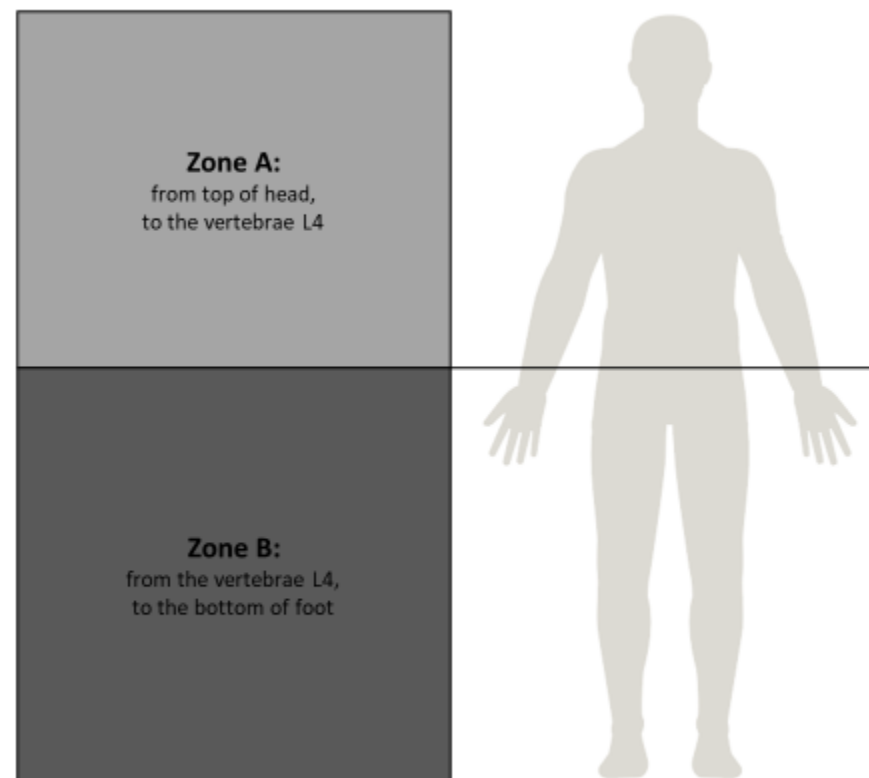


Figure 77

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

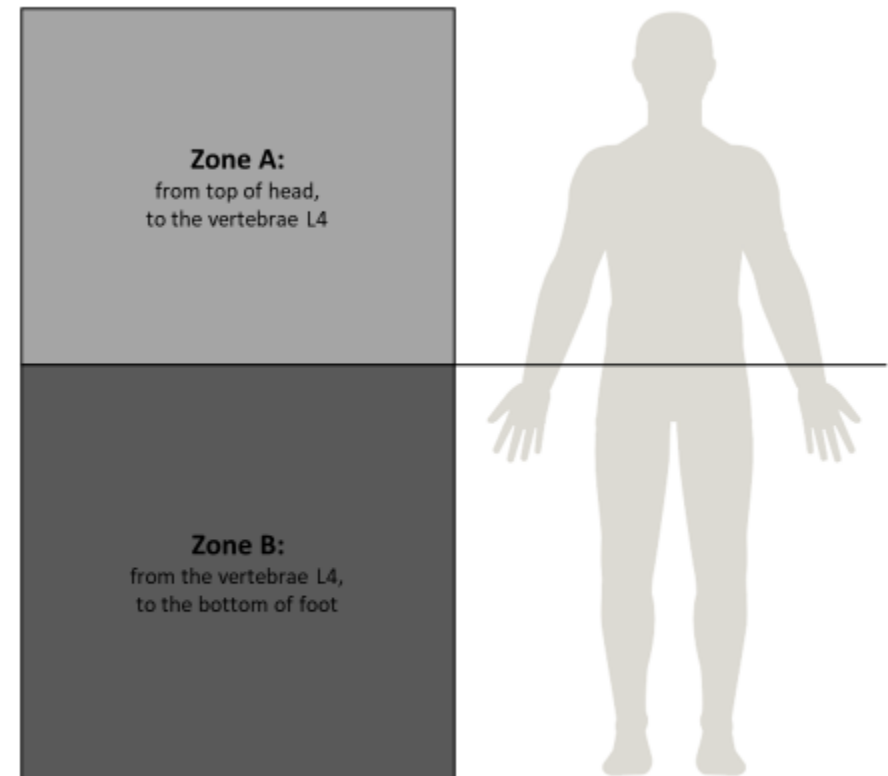


Figure 78

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

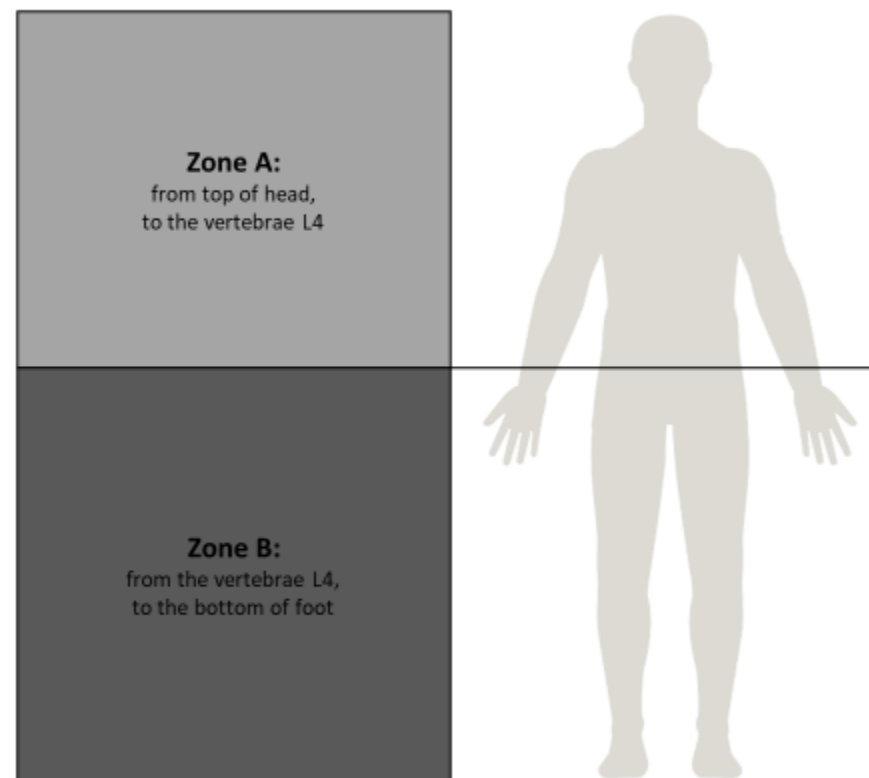


Figure 79



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

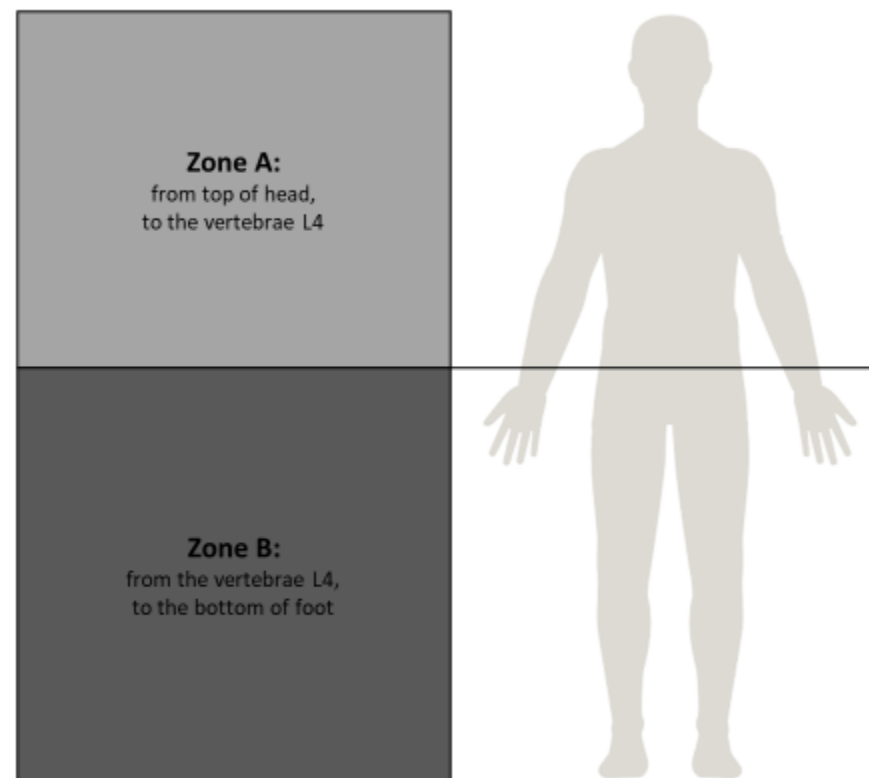


Figure 80



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

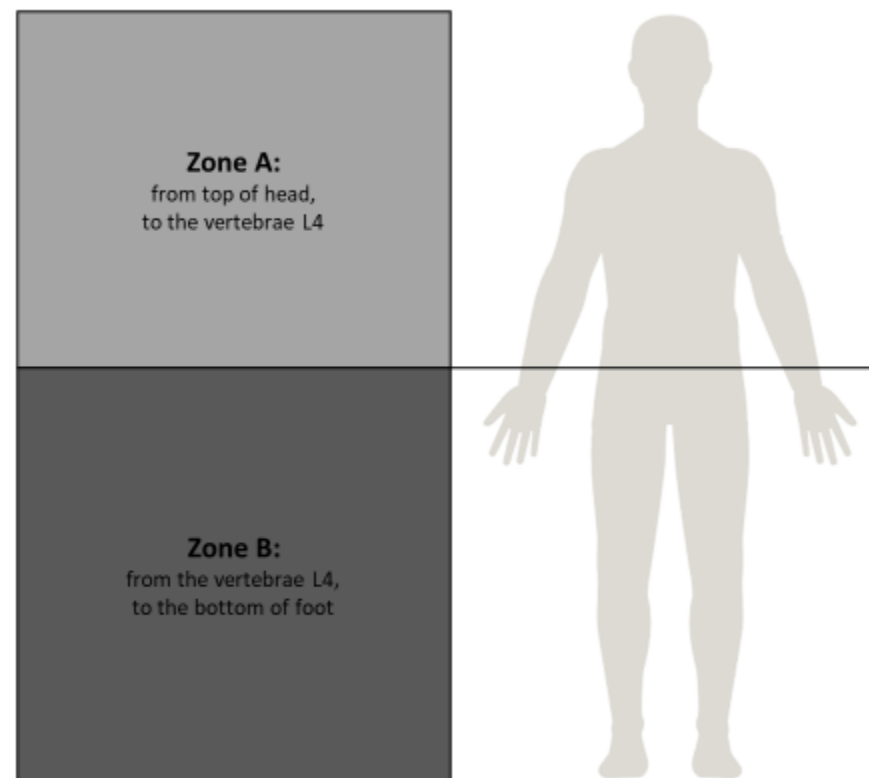


Figure 81

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

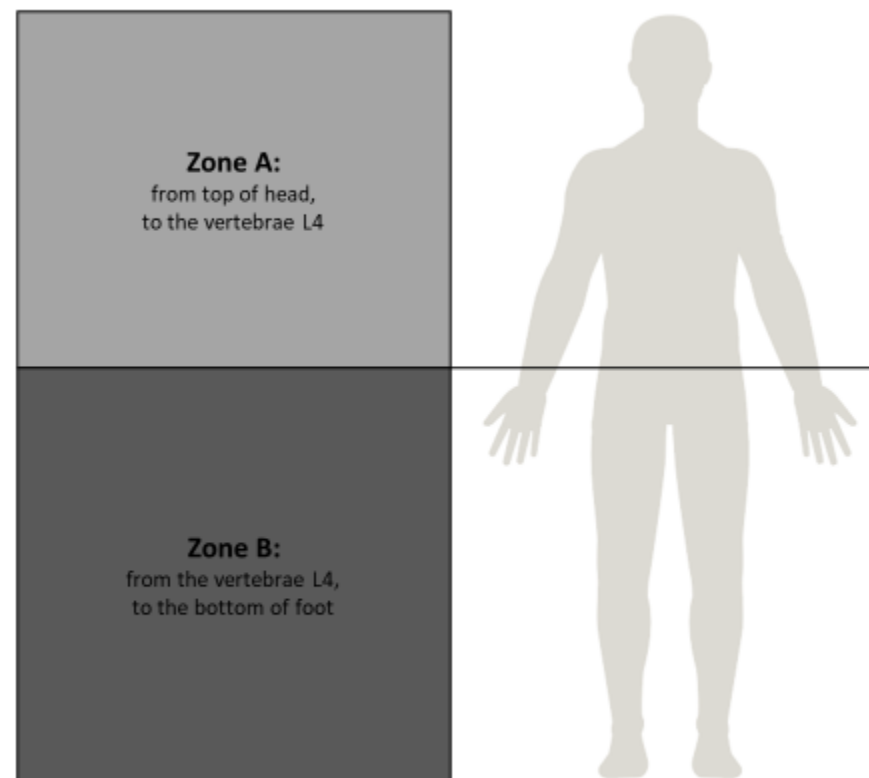


Figure 82

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

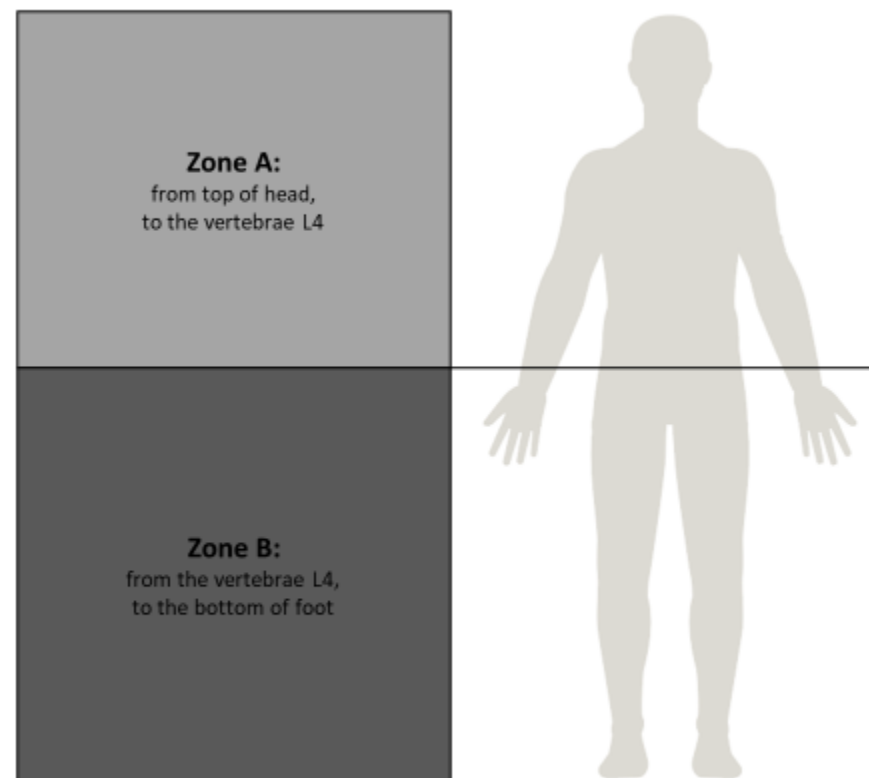


Figure 83

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

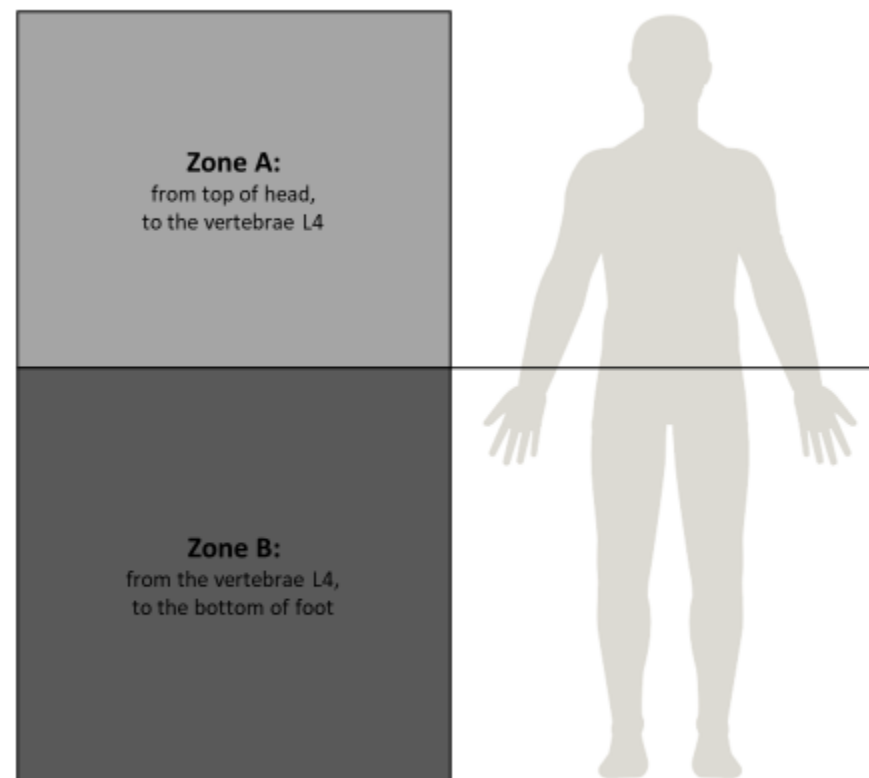


Figure 84

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

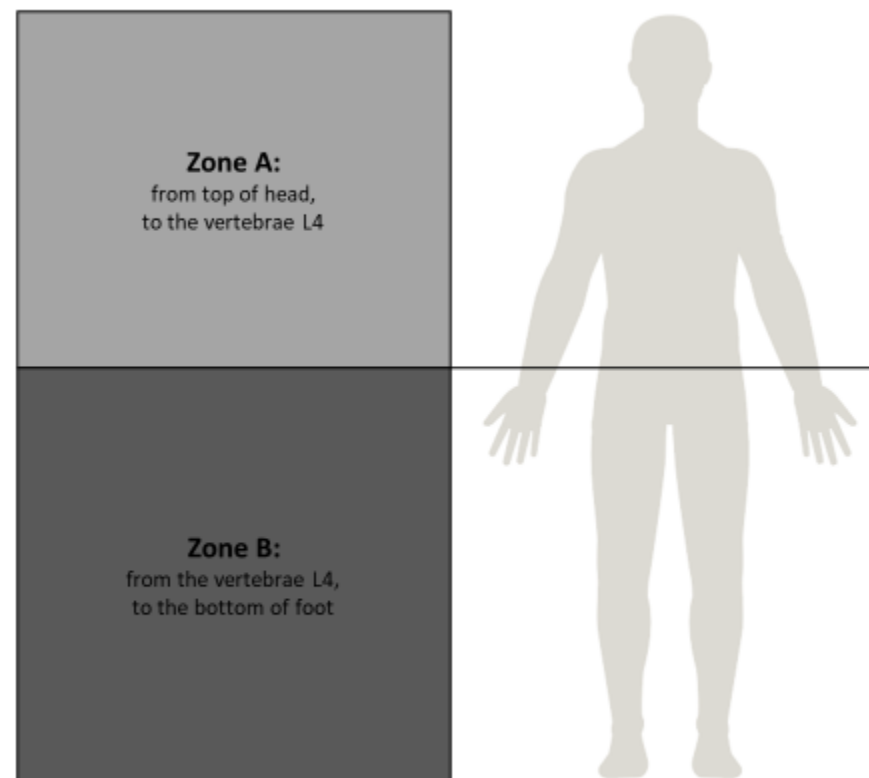


Figure 85

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

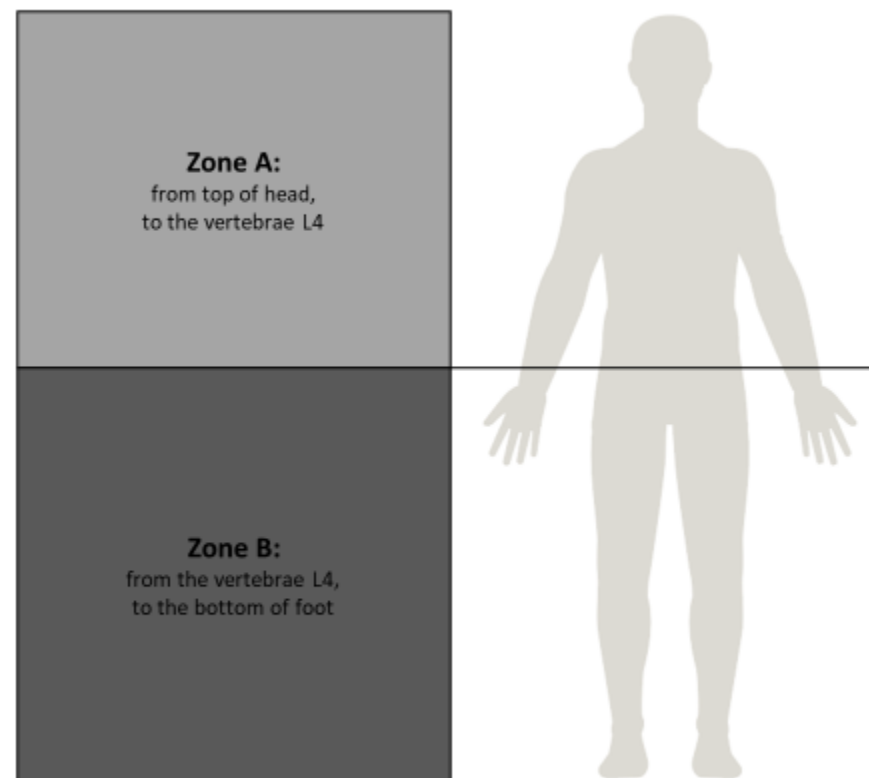


Figure 86

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

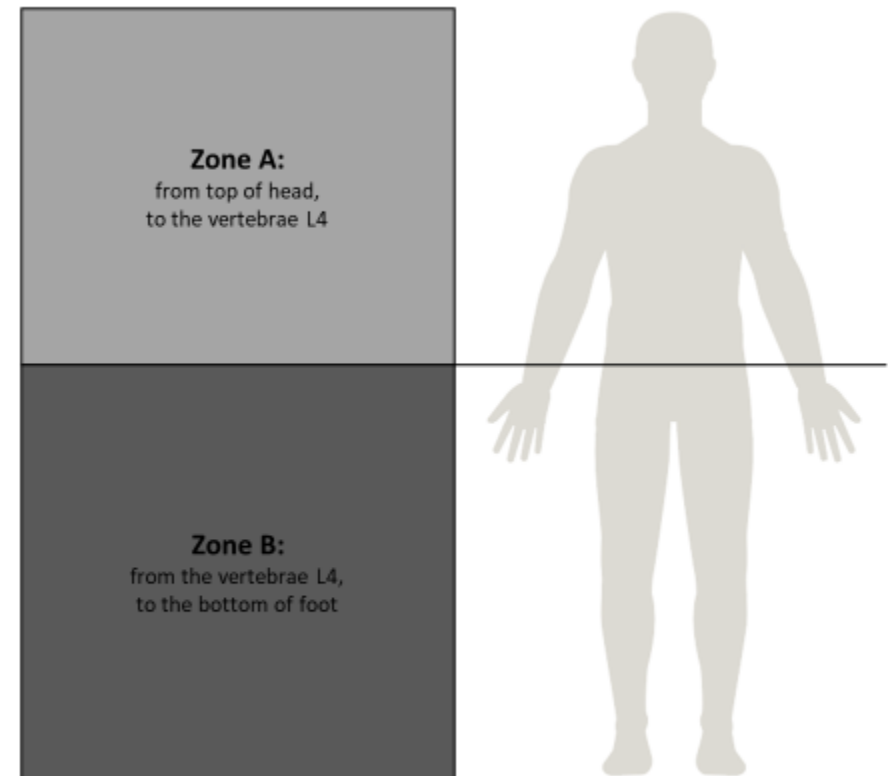


Figure 87



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

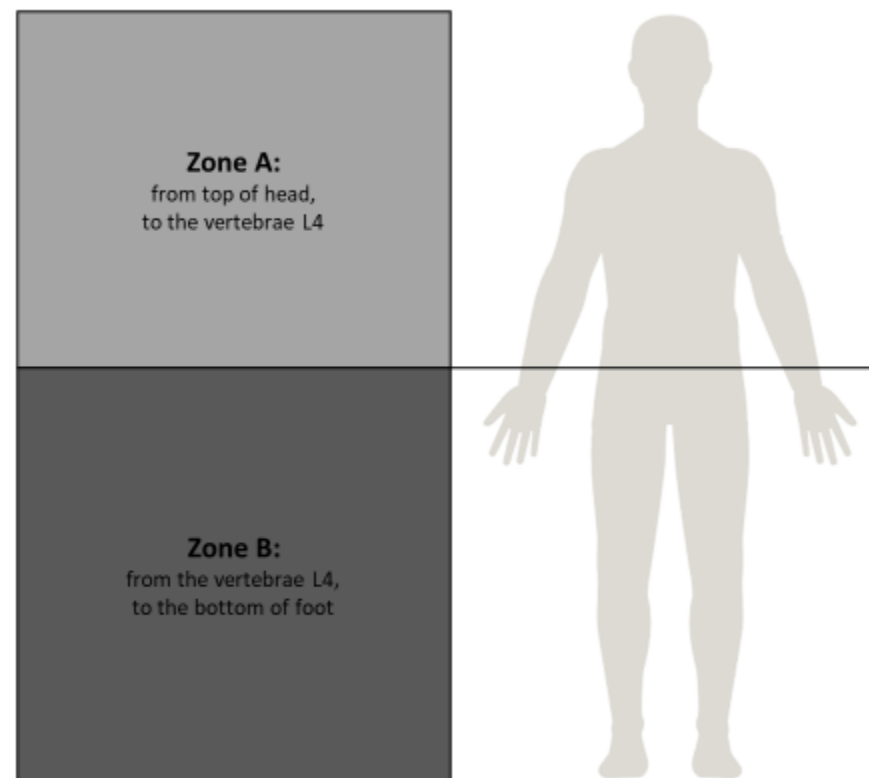


Figure 88



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

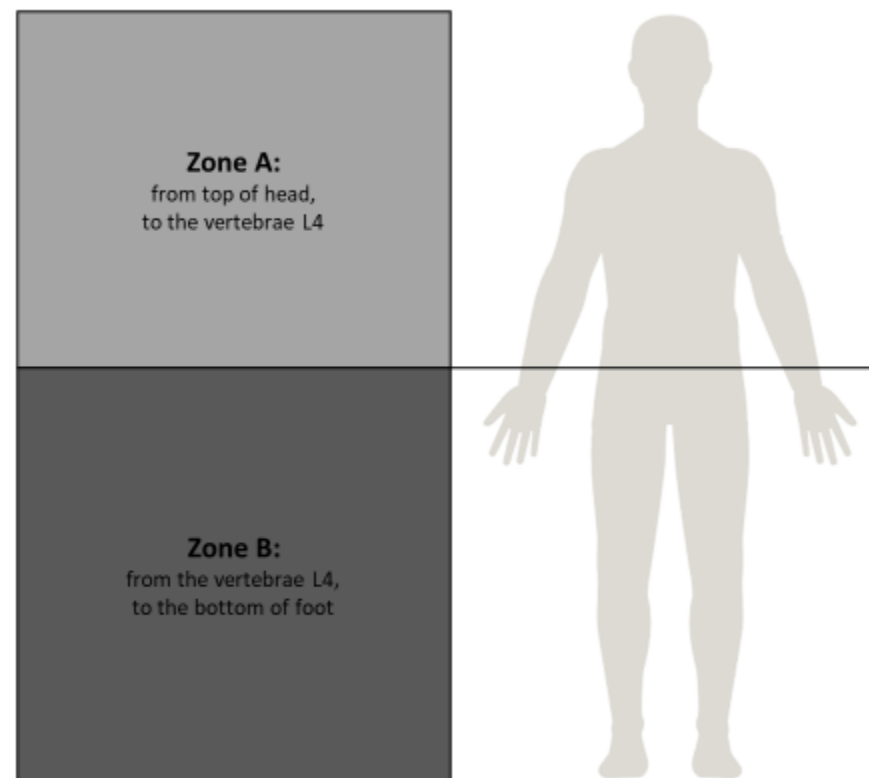


Figure 89

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

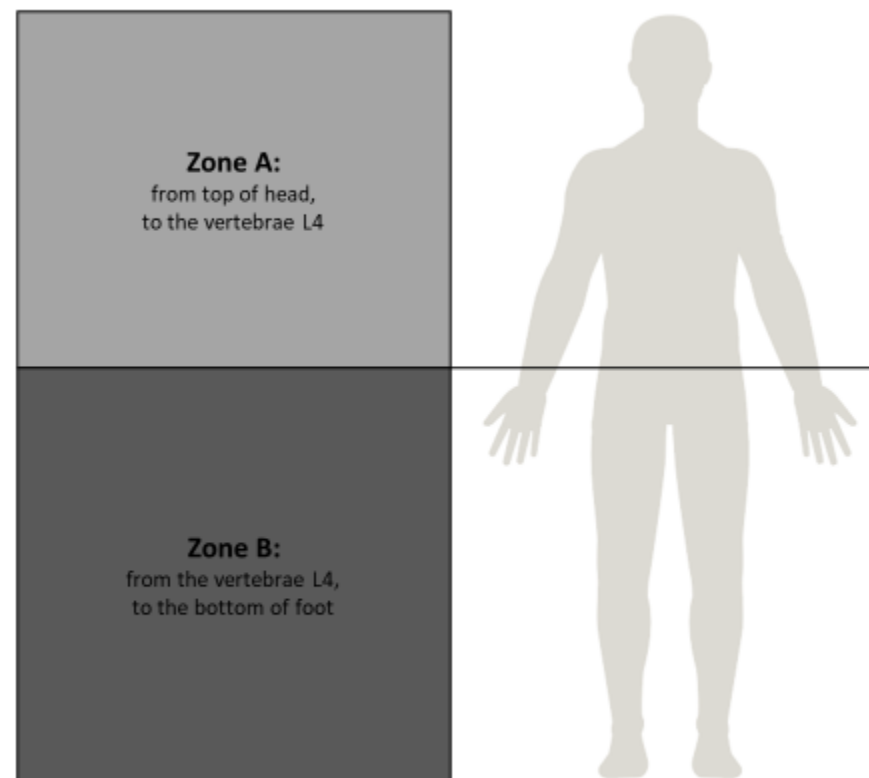


Figure 90

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

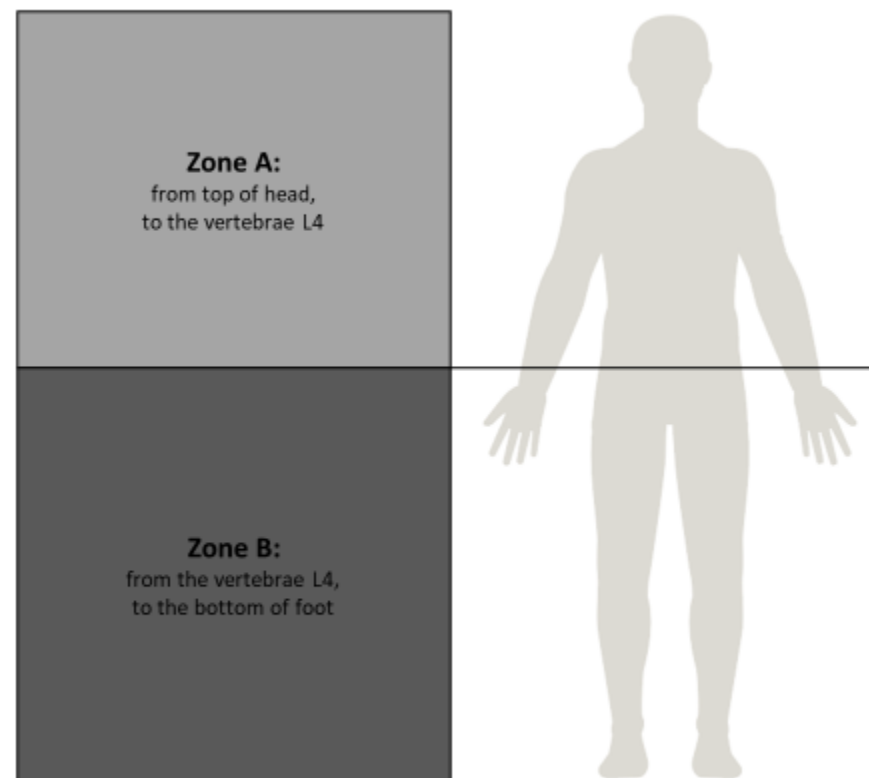


Figure 91

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

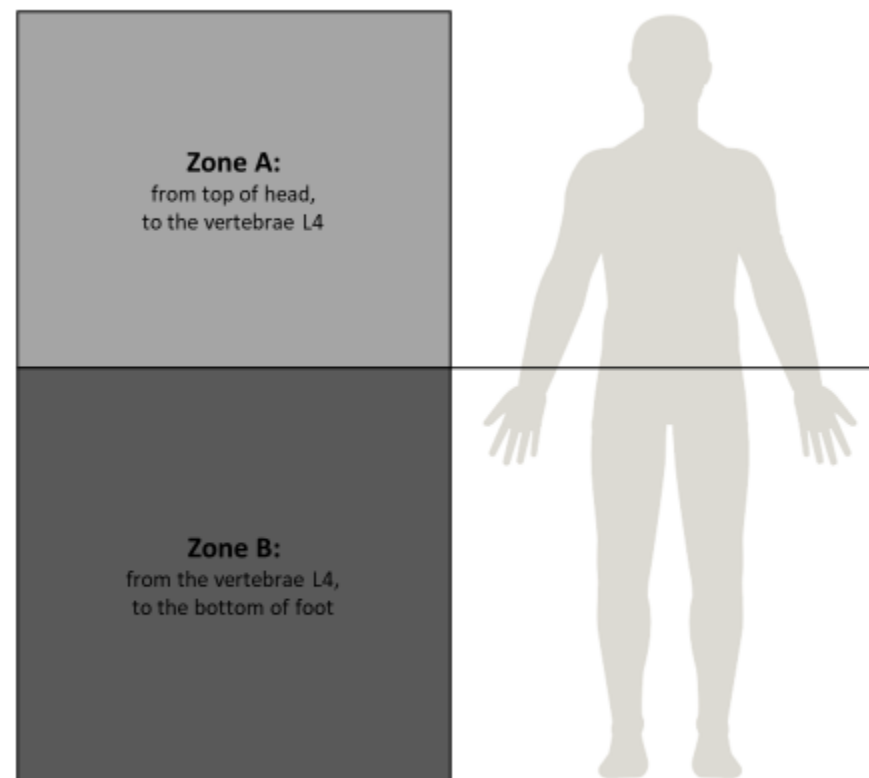


Figure 92

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

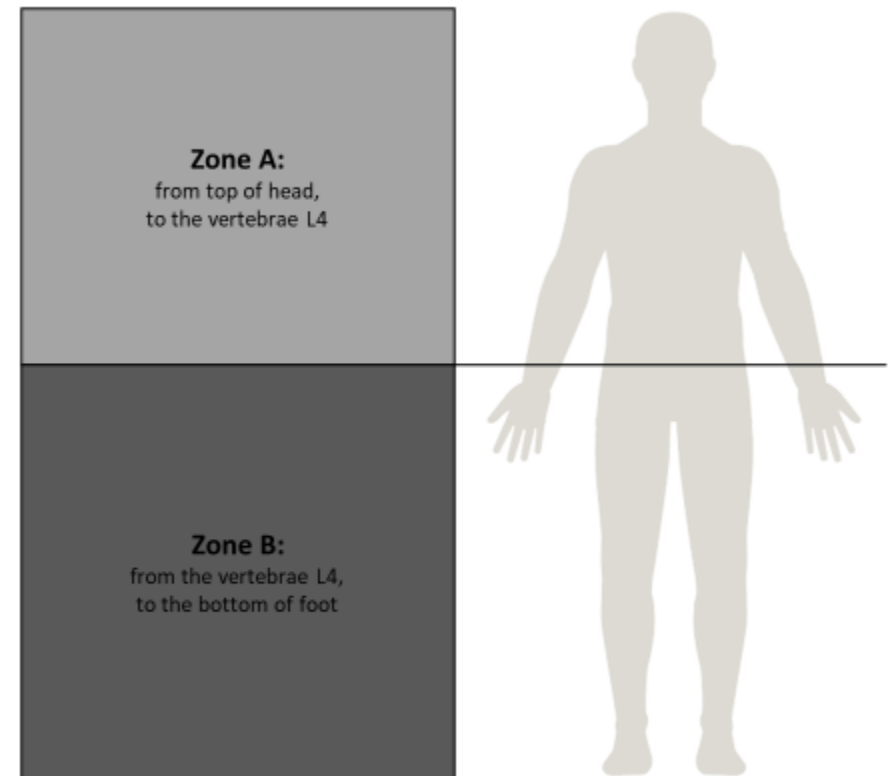


Figure 93

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

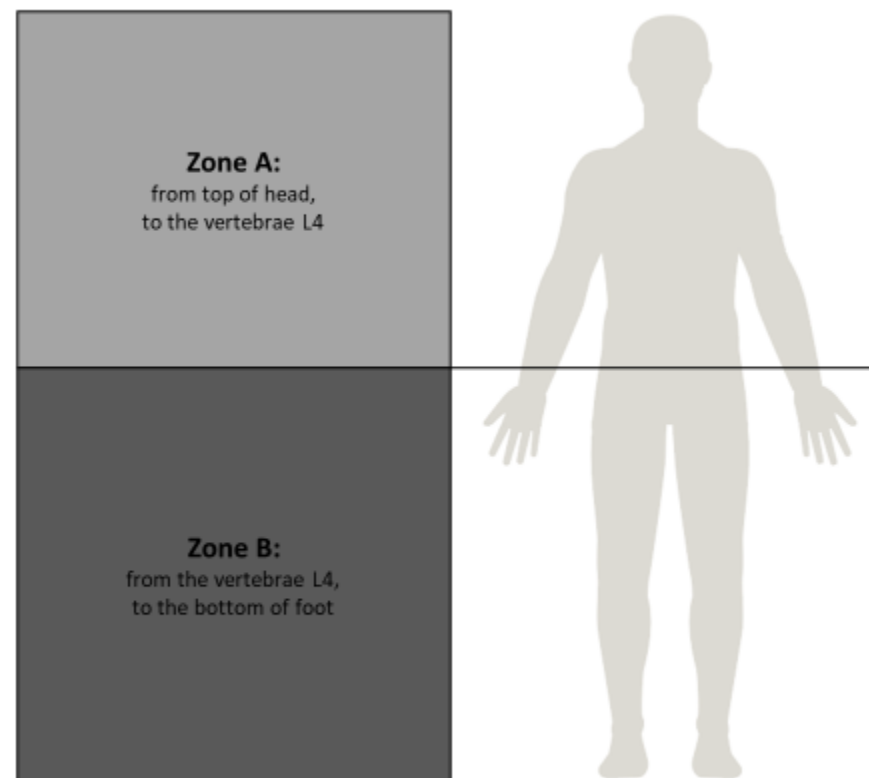


Figure 94

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

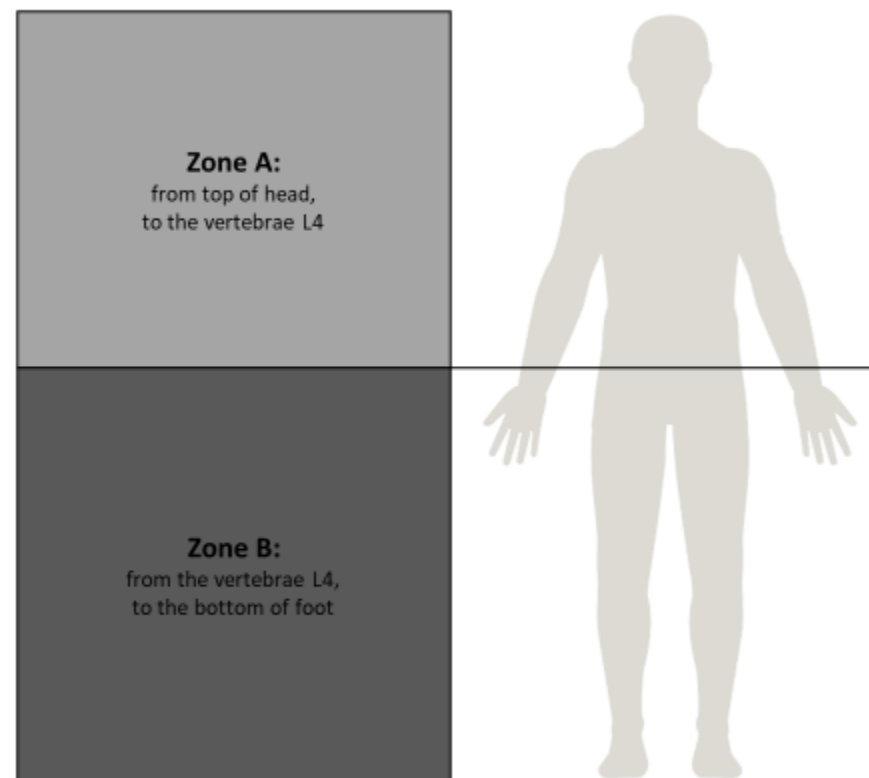


Figure 95



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

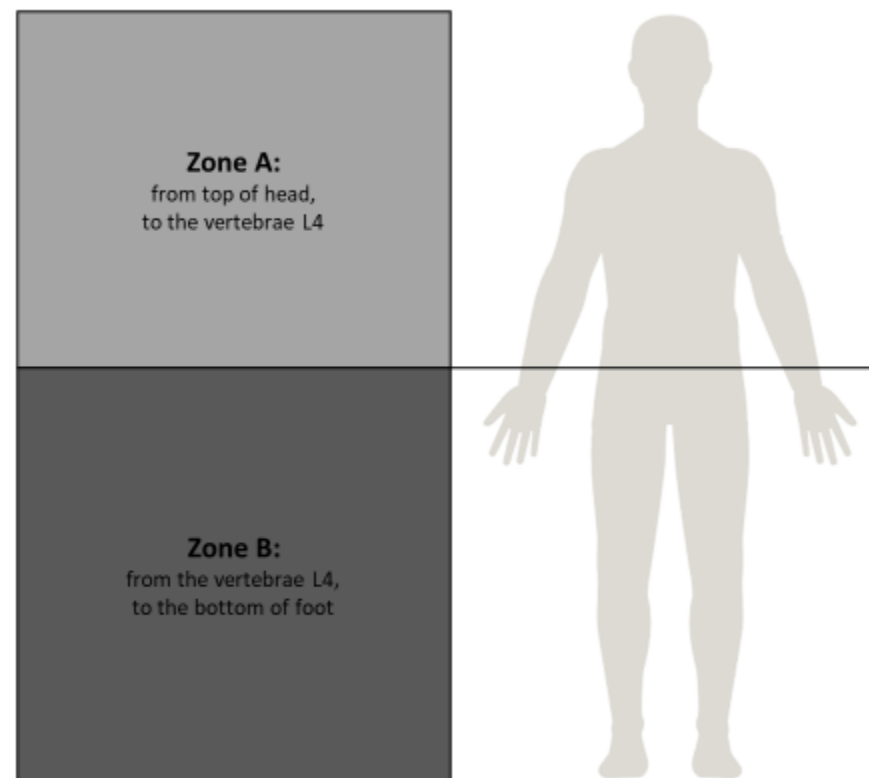


Figure 96



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

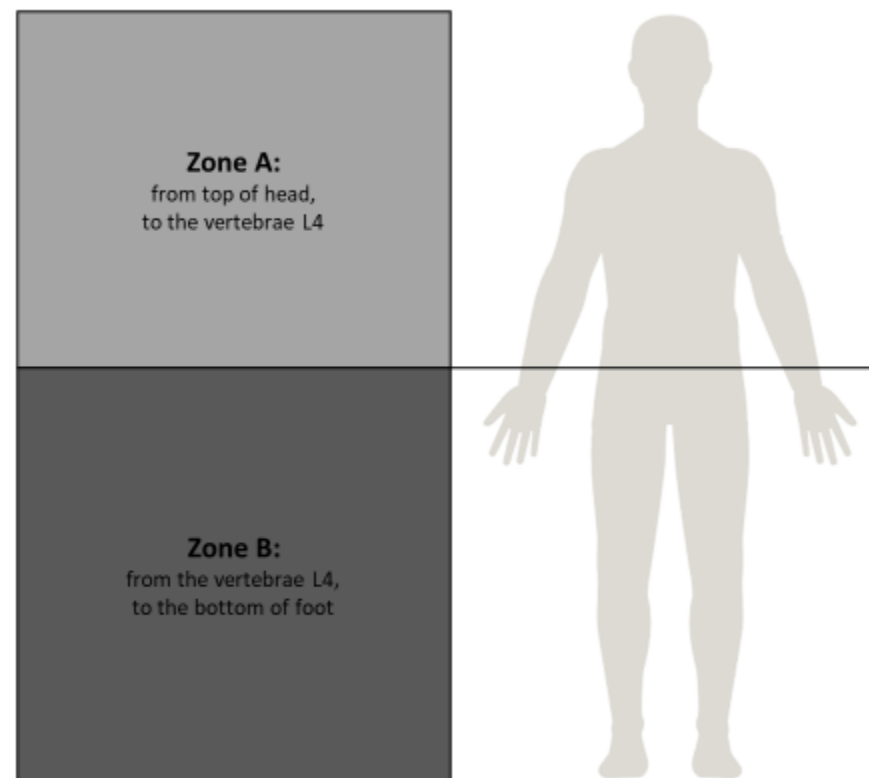


Figure 97

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.0$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

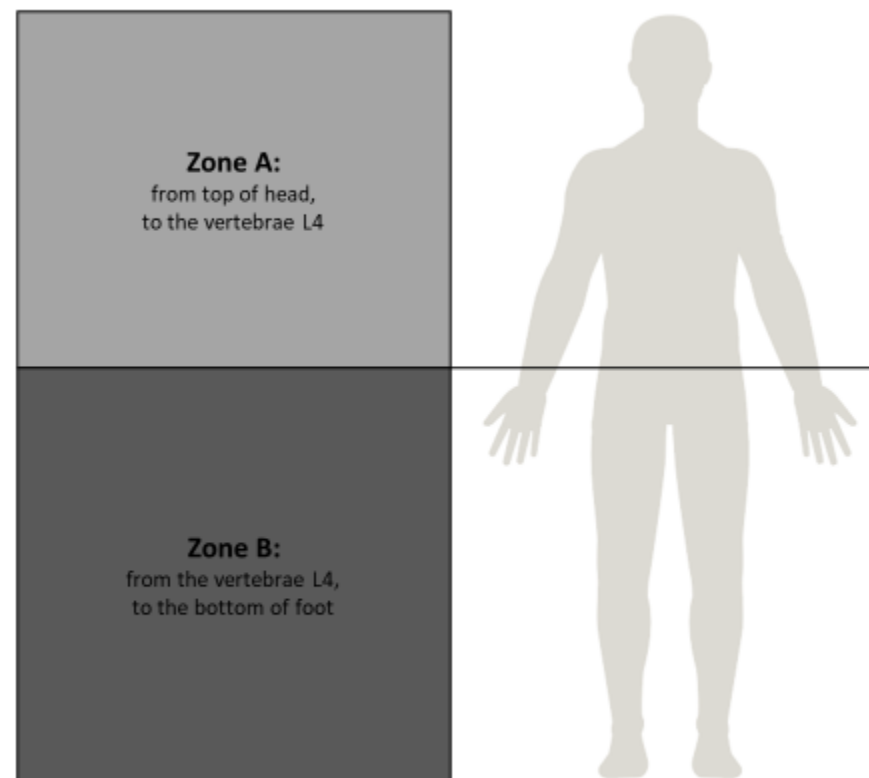


Figure 98

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.0$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

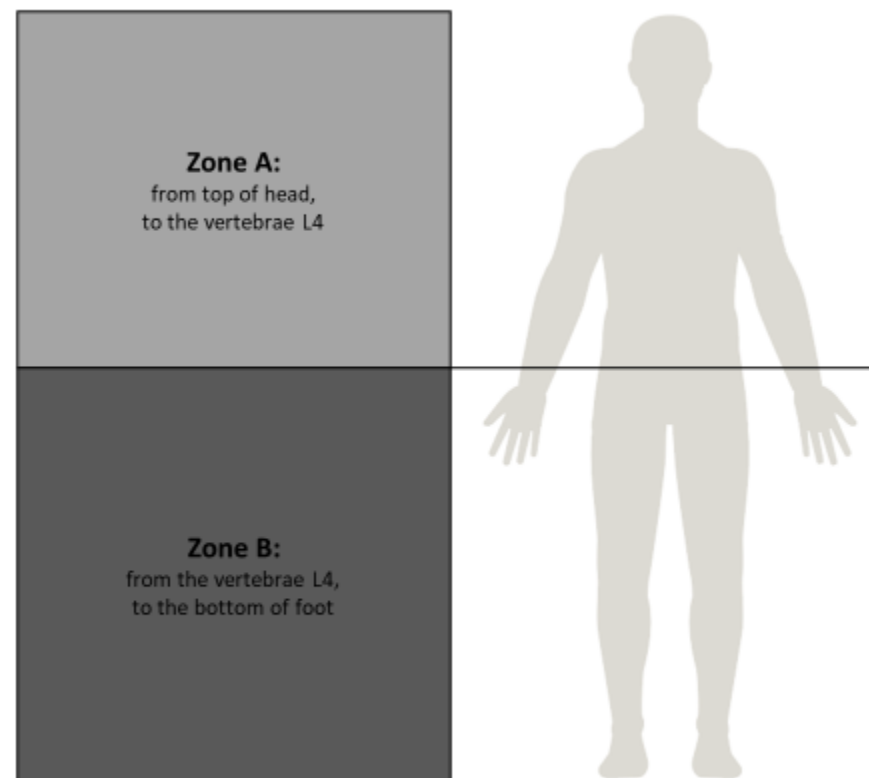



Figure 99

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.0$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

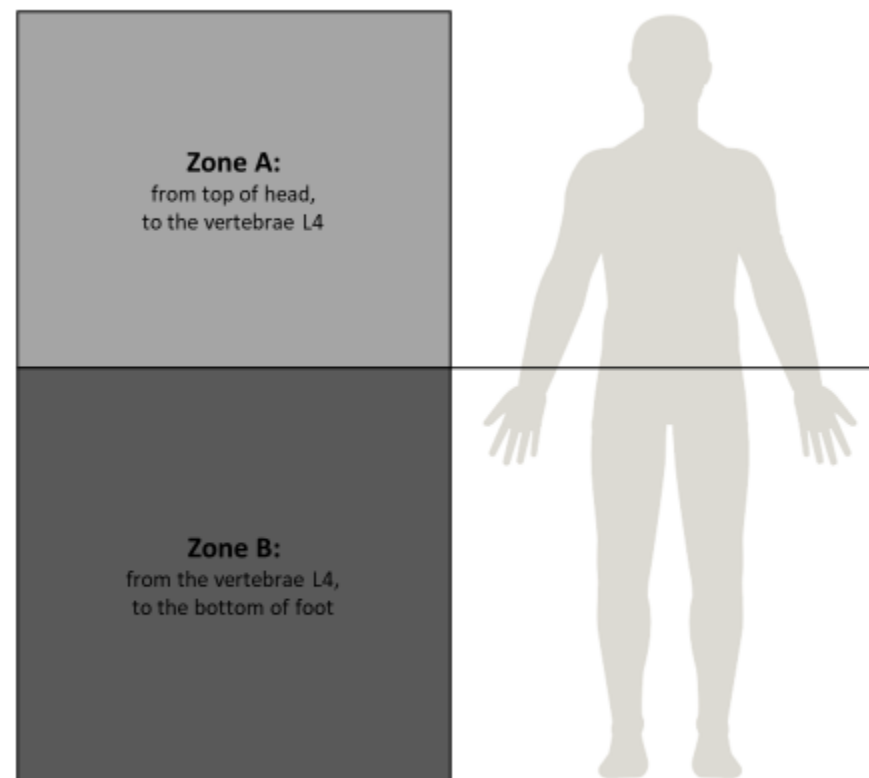


**Figure 100**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.0$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

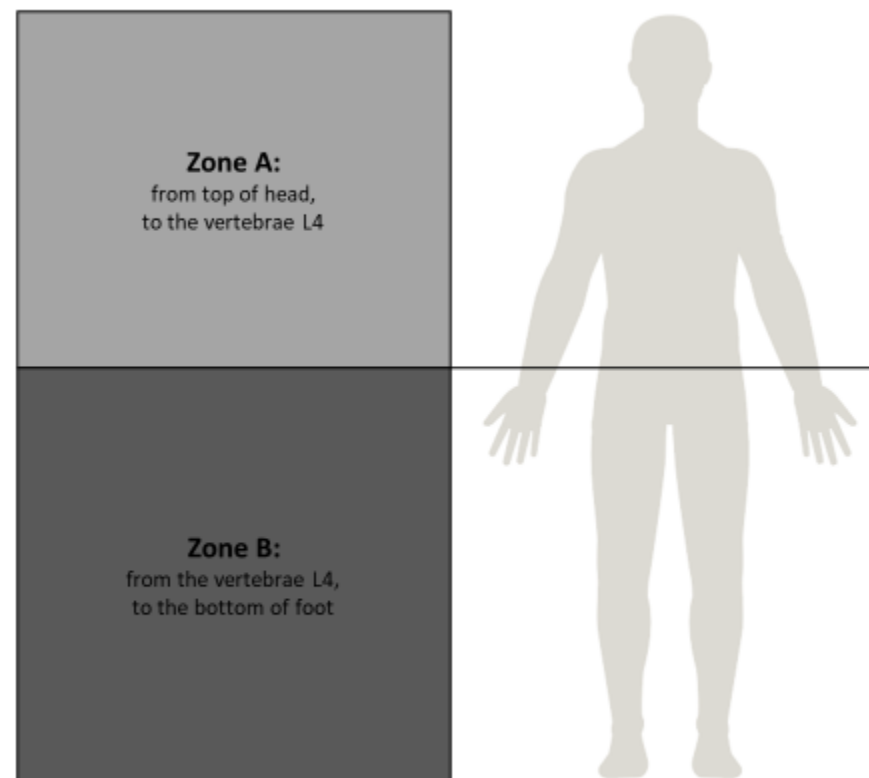


**Figure 101**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.1$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

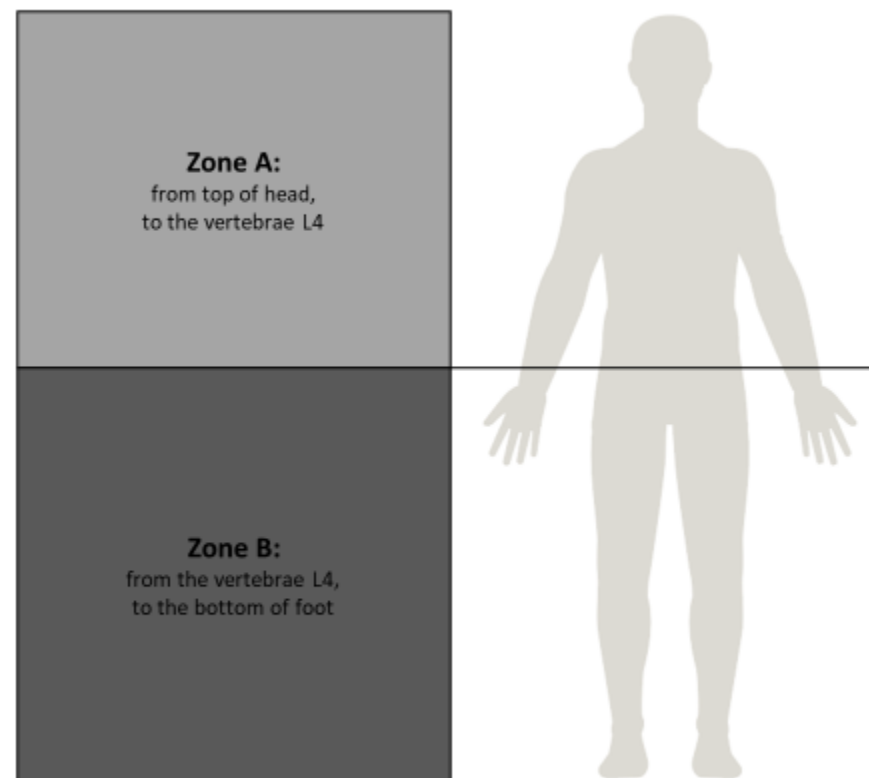


**Figure 102**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.2$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

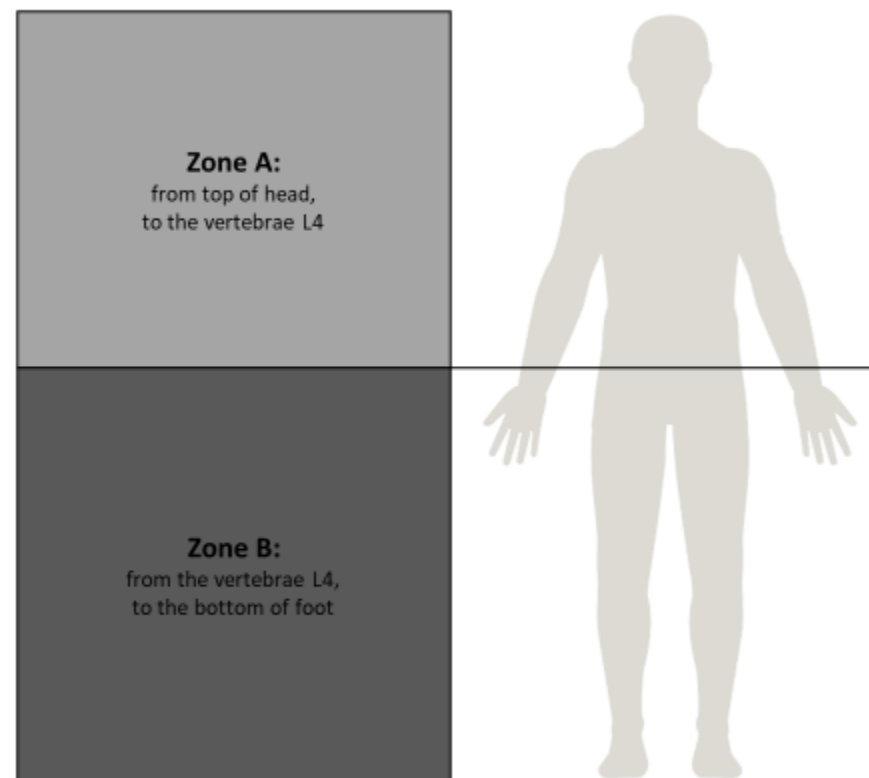

**Figure 103**




**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.2$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

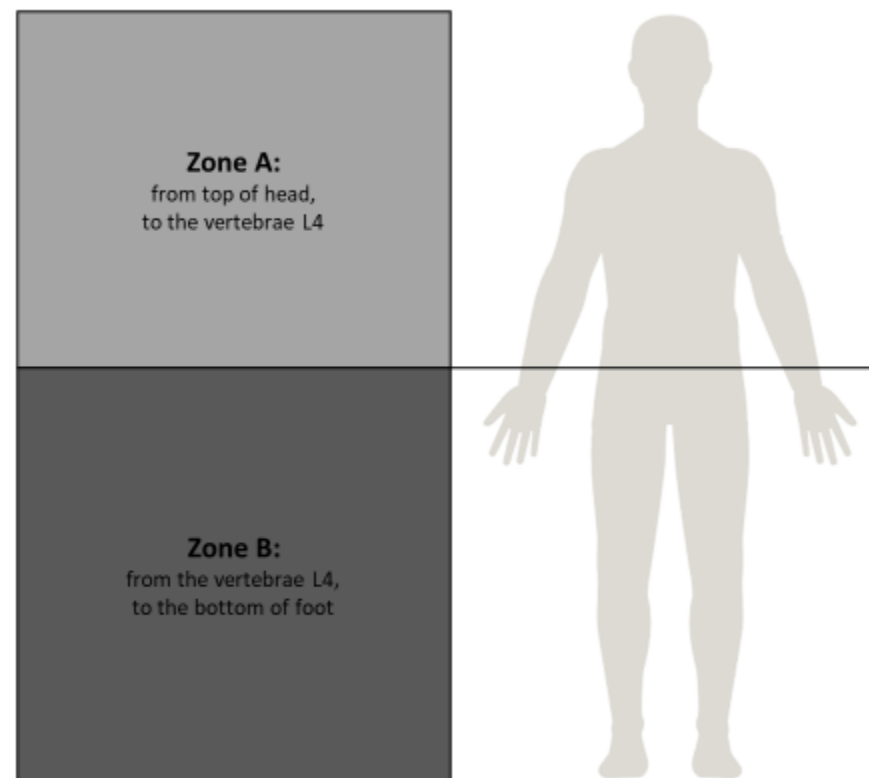**Figure 104**




**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.3$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

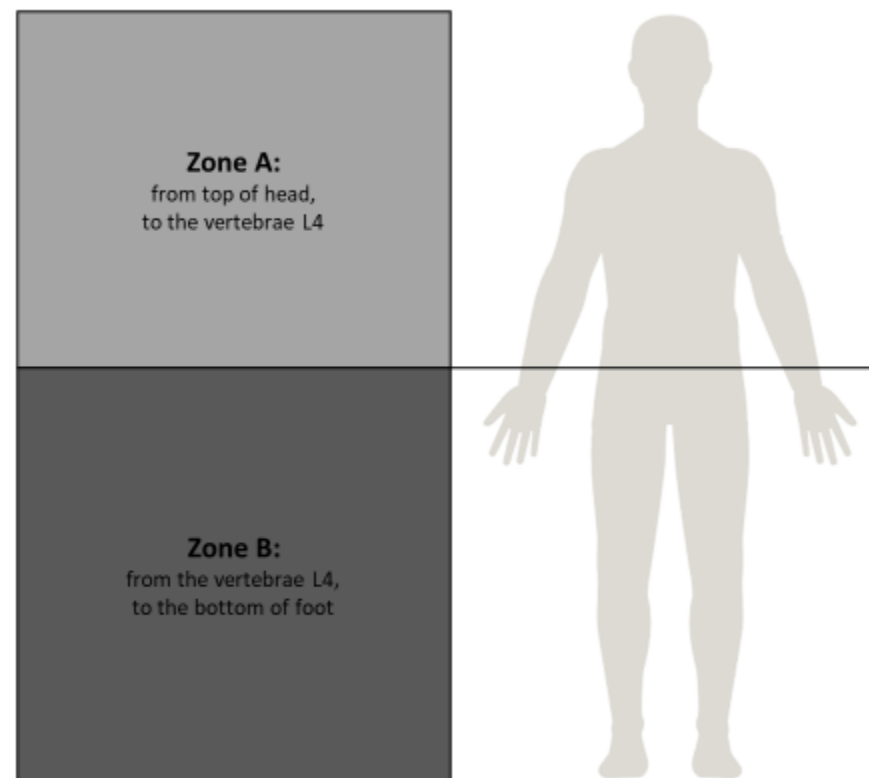
**Figure 105**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.4$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

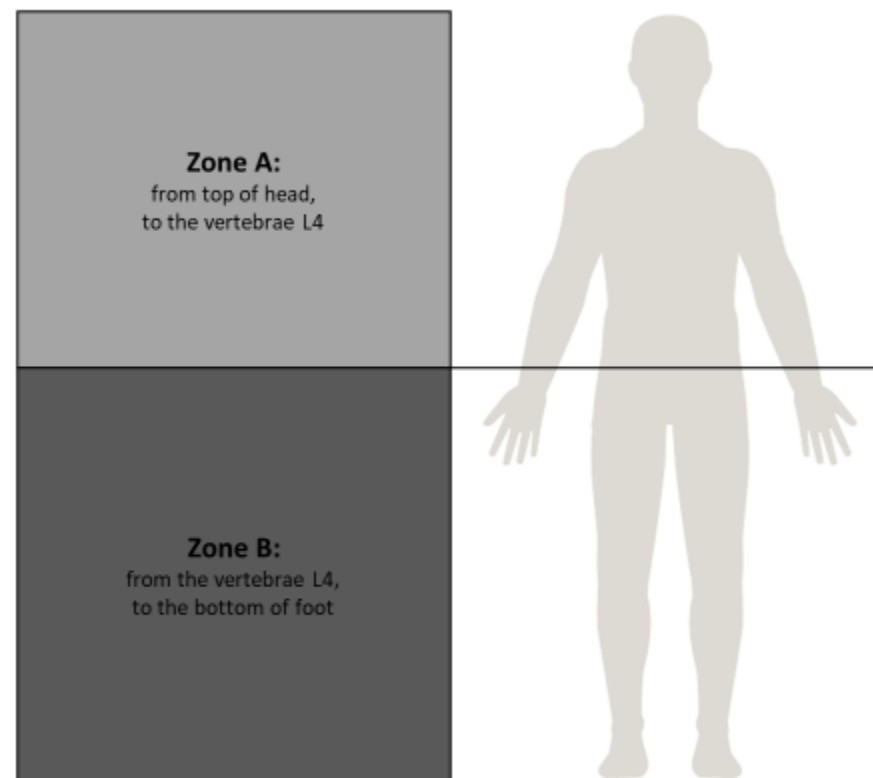**Figure 106**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.4$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

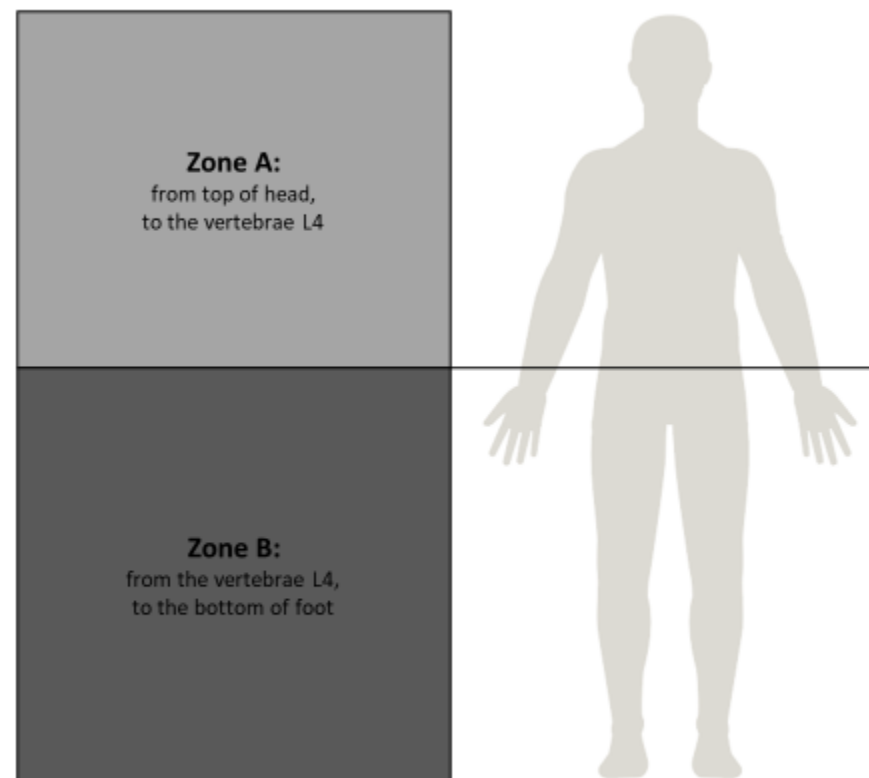



Figure 107

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.5$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

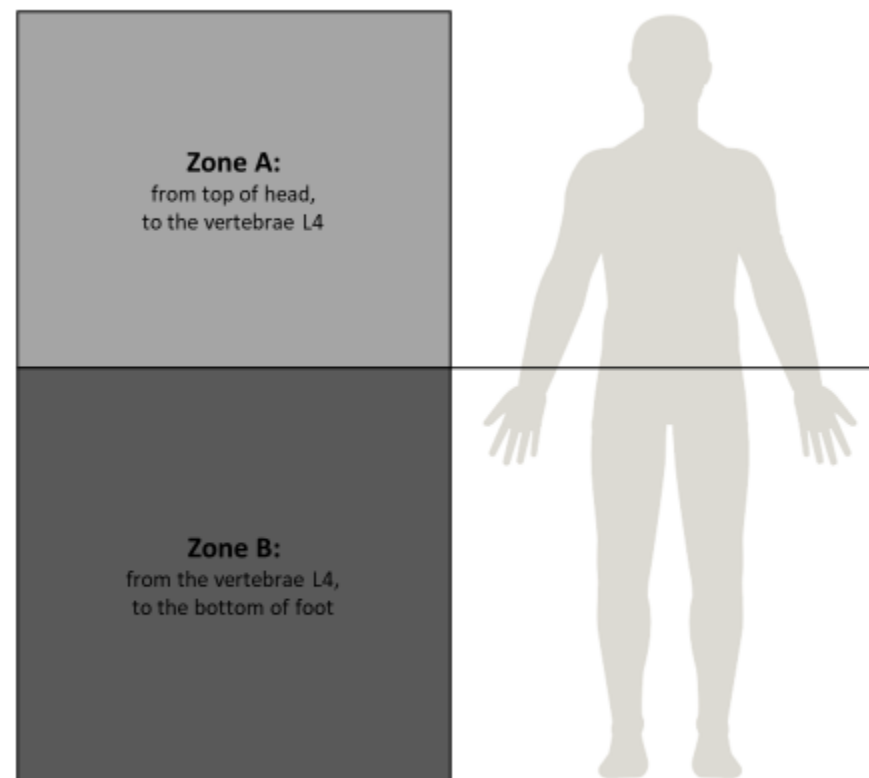
**Figure 108**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.5$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

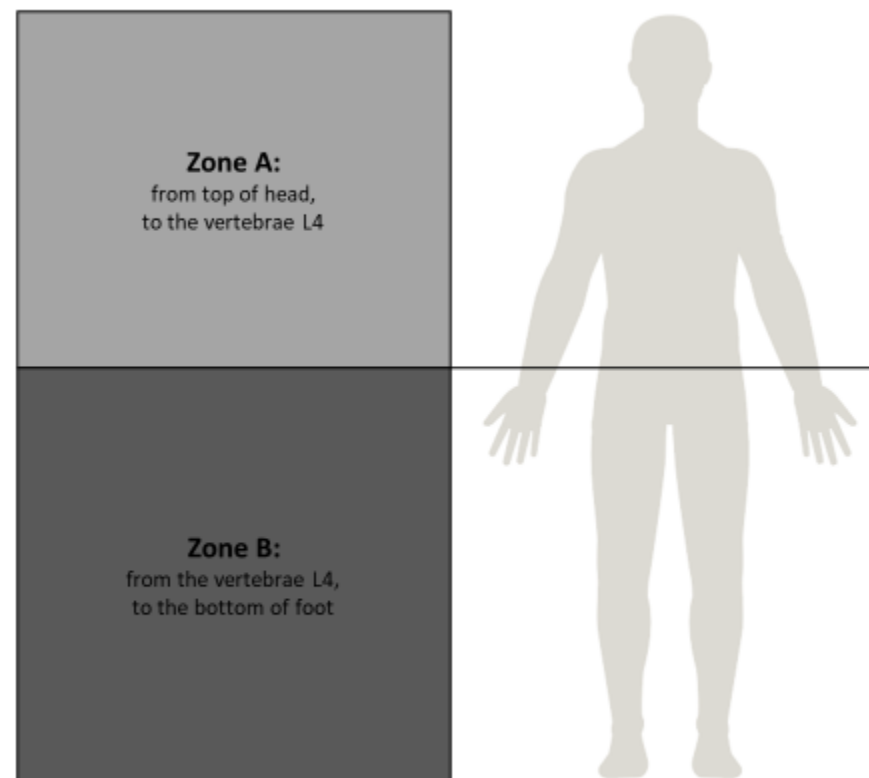
**Figure 109**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.7$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

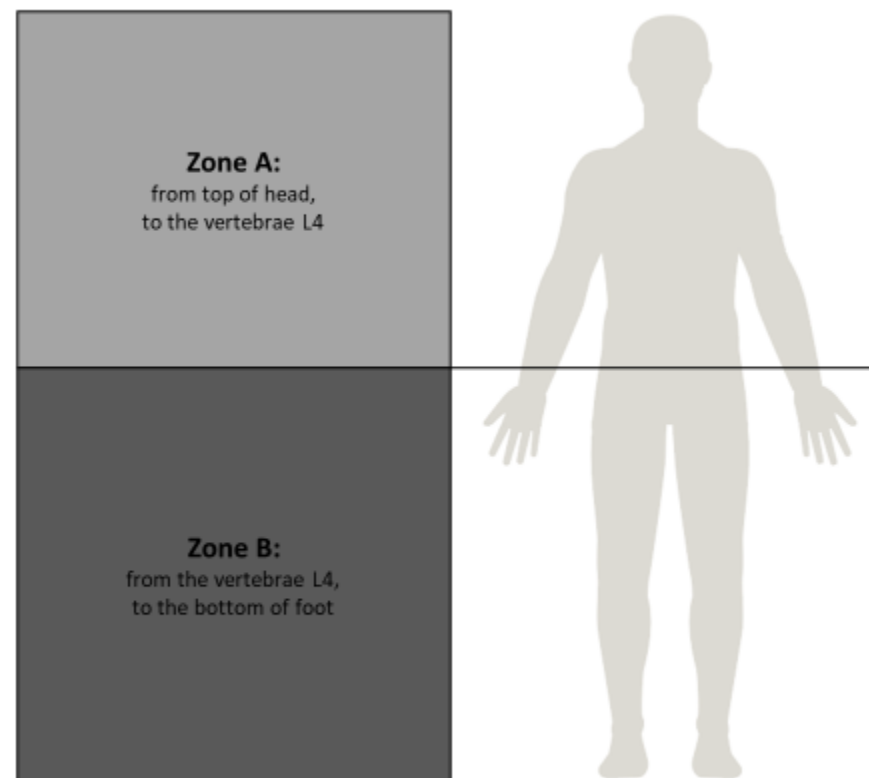


**Figure 110**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.8$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

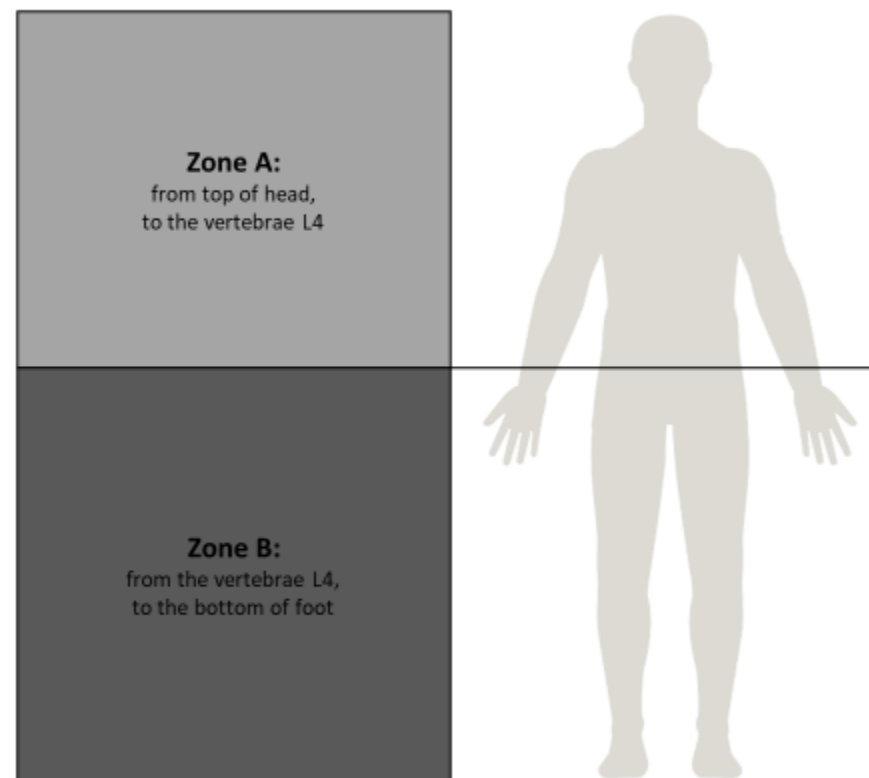

**Figure 111**




**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.8$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

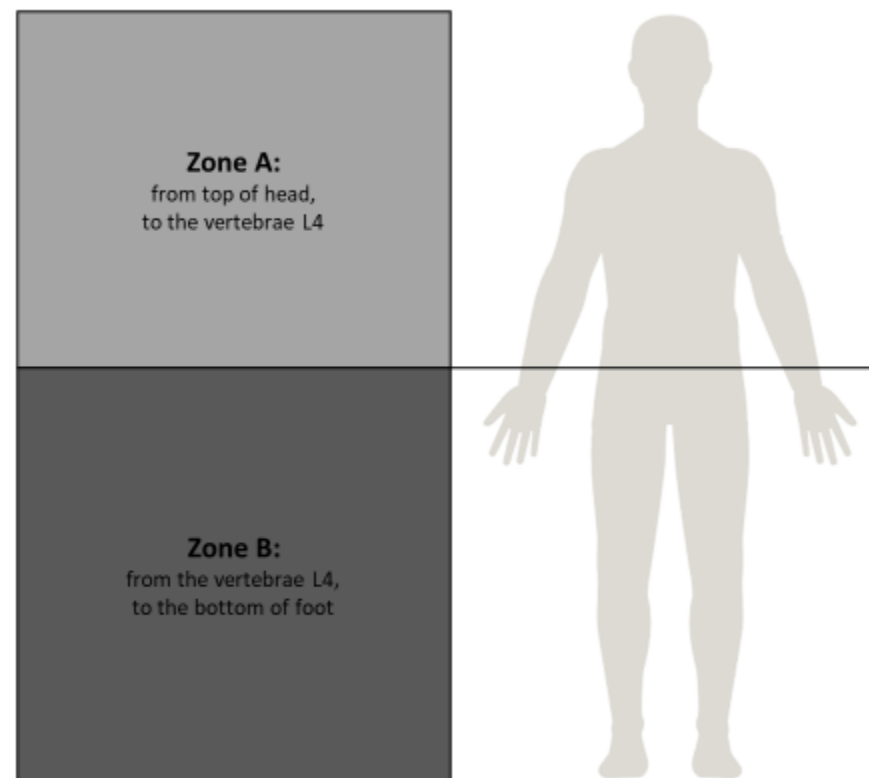

**Figure 112**




**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.0$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

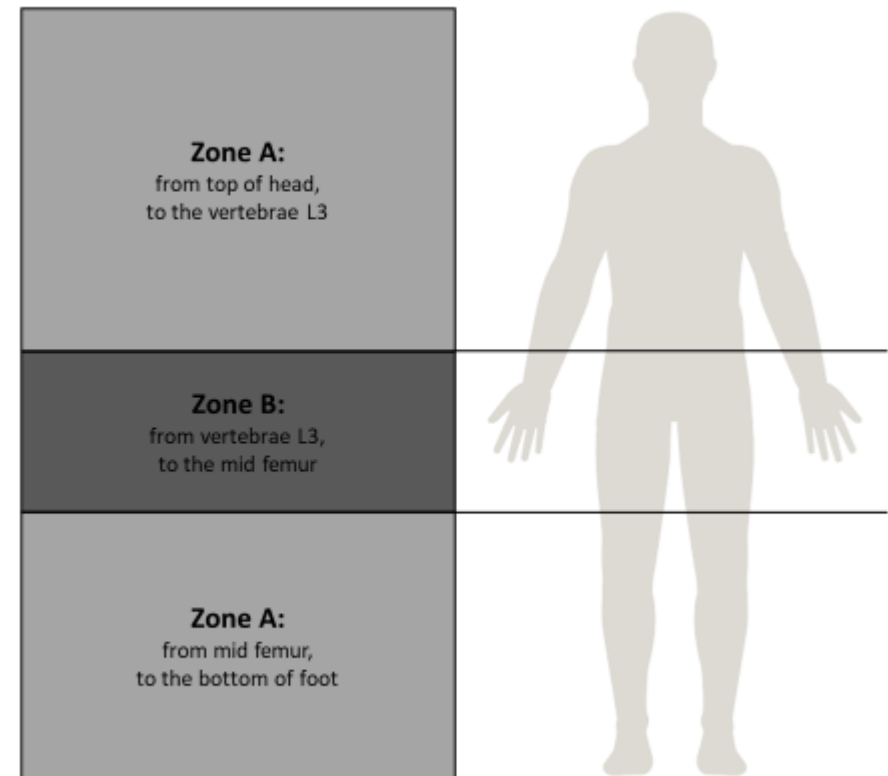
**Figure 113**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.4$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

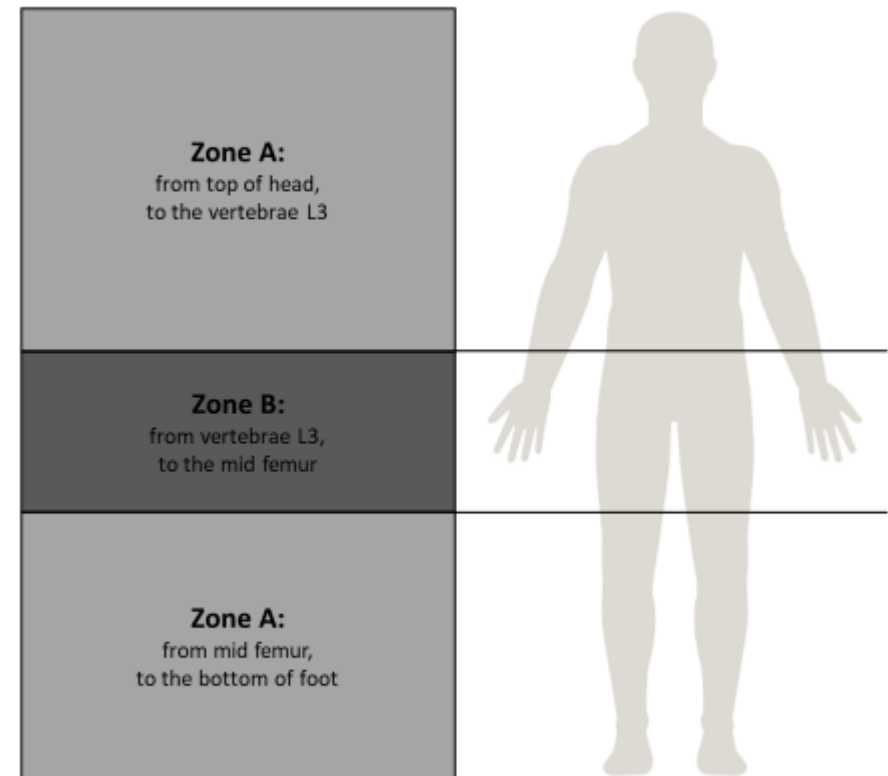**Figure 114**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.6$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

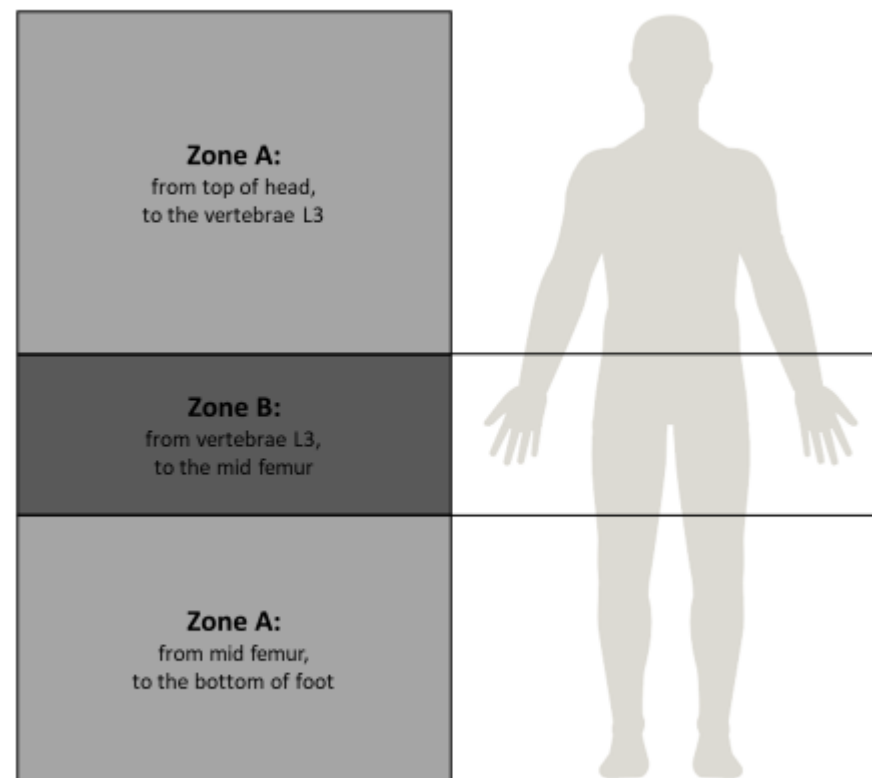



Figure 115

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.3$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

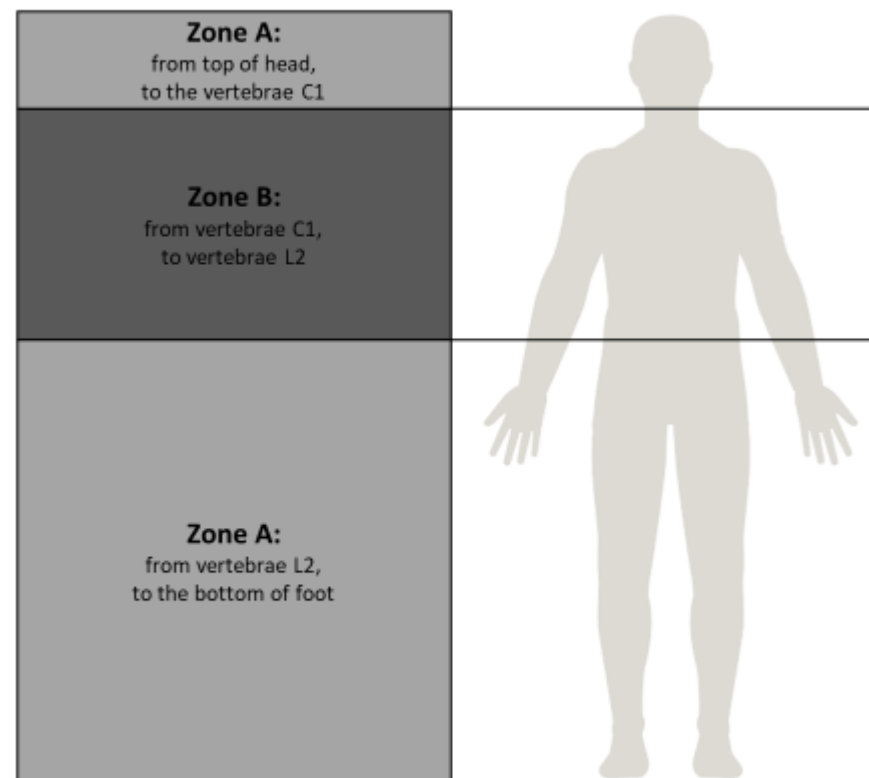
**Figure 116**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

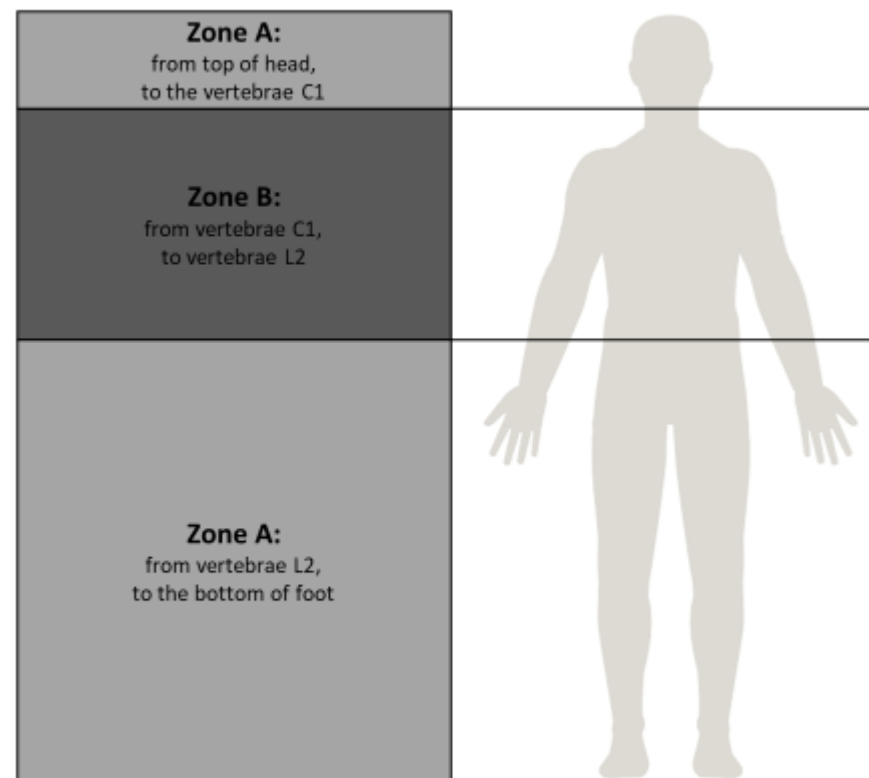**Figure 117**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

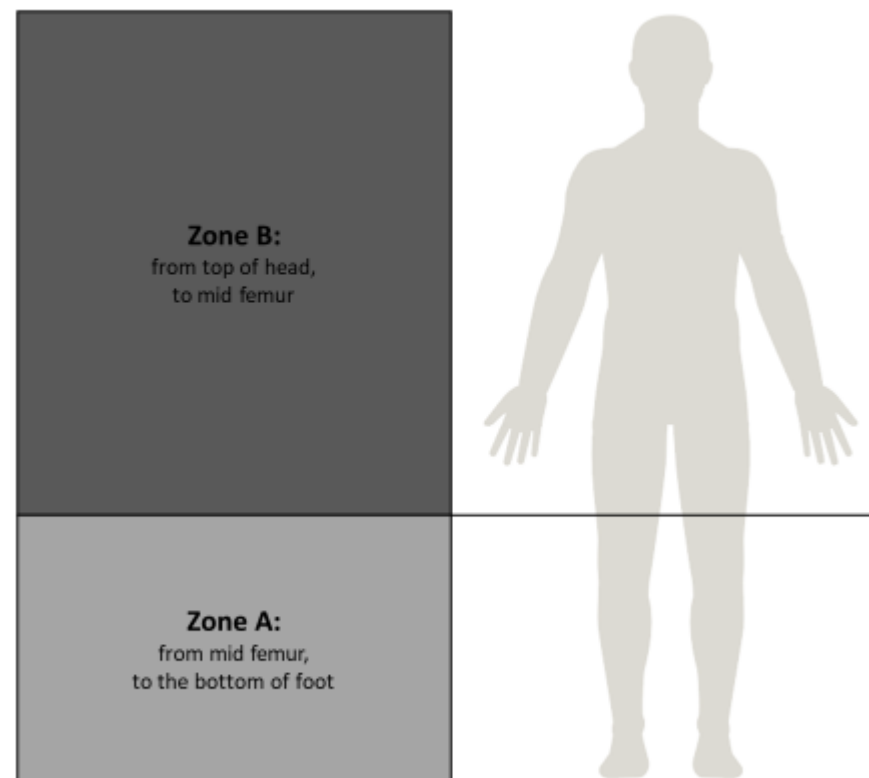



Figure 118

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

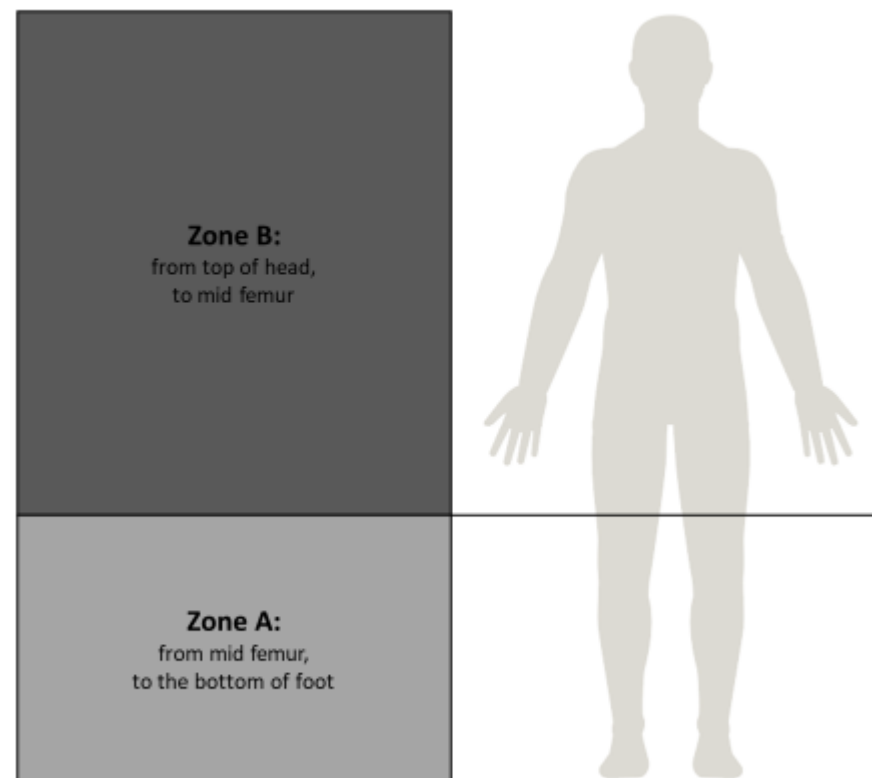

**Figure 119**



**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

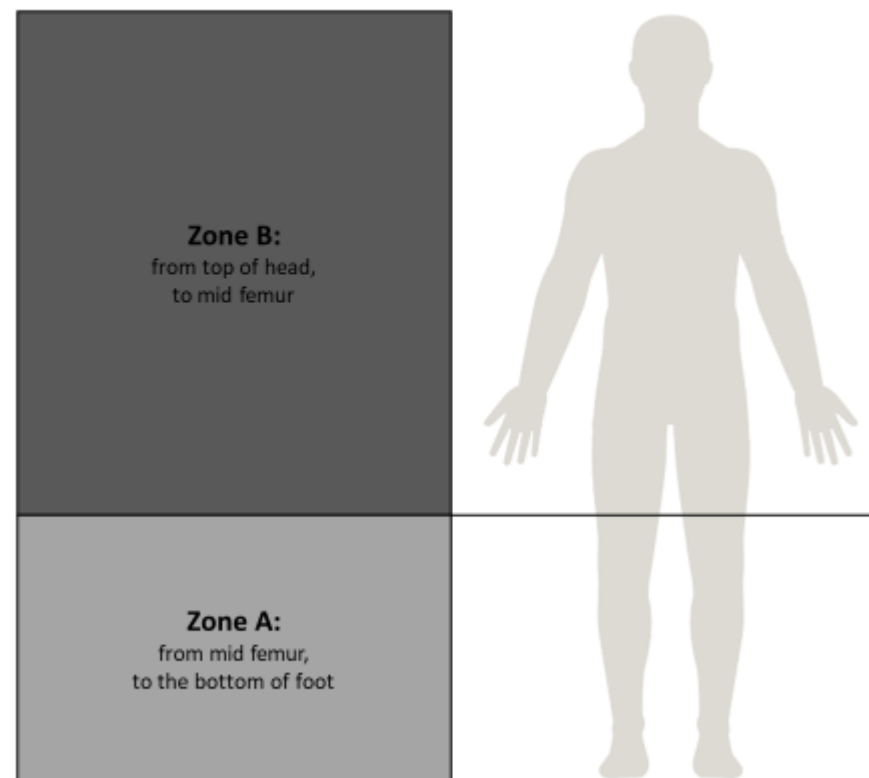


Figure 120




**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> Whole Body SAR $\leq 1.3$ W/kg
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

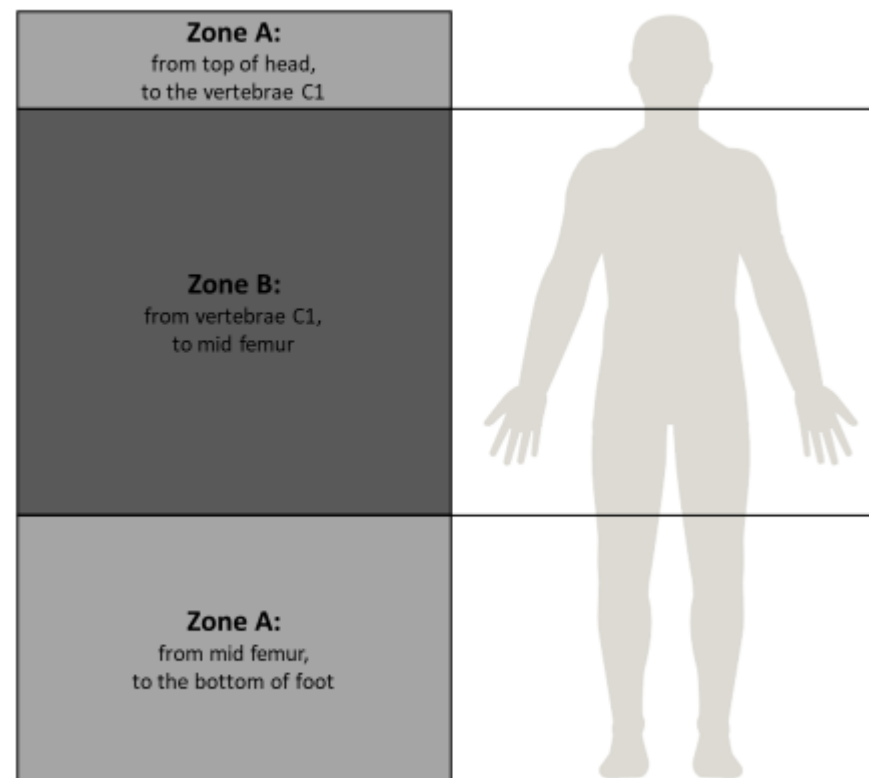
**Figure 121**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.

**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

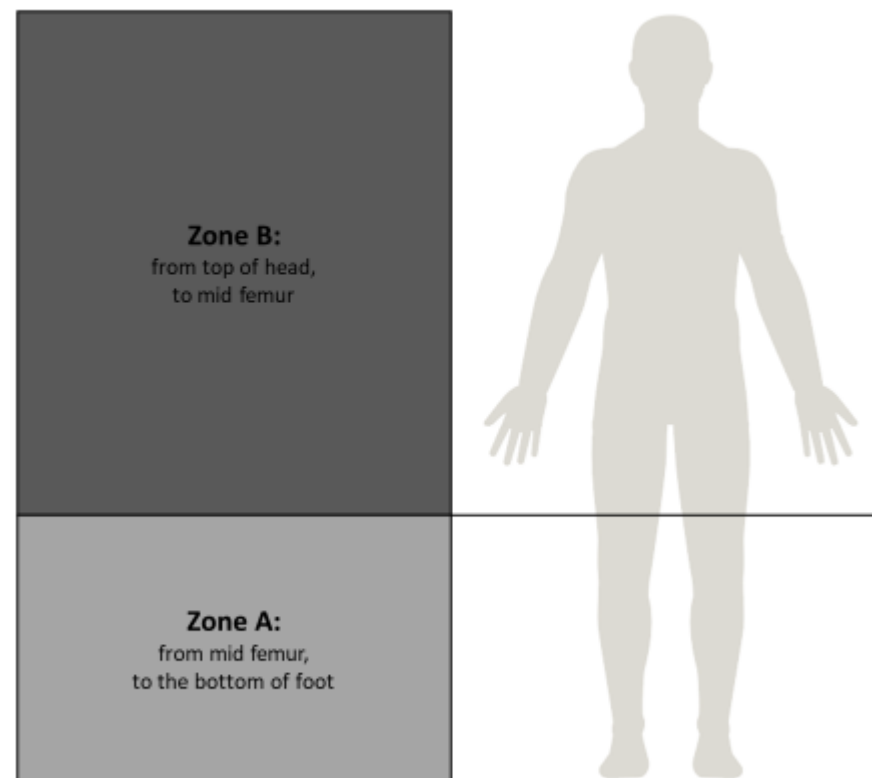


**Figure 122**

**MR Conditional****MRI Safety Information**

For Whole-Body MR Examinations: A person implanted with the Nalu Neurostimulation System may be safely scanned anywhere in the body at 1.5 T under the following conditions. Failure to follow these conditions may result in injury. NOTE: This label is only applicable to certain implant codes and/or implant code combinations. Refer to the guide on page 11 for directions on how to generate a patient's implant code and corresponding MR Conditionality.

Parameter	Condition
Device Name	Nalu Neurostimulation System
Device Configuration	Stimulation OFF, no external devices
Static Magnetic Field Strength ( $B_0$ )	1.5 T
MR Scanner Type	Cylindrical
$B_0$ Field Orientation	Horizontal
Maximum Spatial Field Gradient	20 T/m (2000 gauss/cm)
Maximum Gradient Slew Rate	200 T/m/s per axis
RF Excitation	Circularly Polarized (CP)
RF Transmit Coil Type	Volume Body RF Coil
Receive Coil Type	Any
RF Conditions	<b>For Zone A:</b> Normal Operating Mode (Whole-Body SAR $\leq 2$ W/kg) <b>For Zone B:</b> MR Unsafe, do not scan in this region
Scan Duration	Scan for up to 30 minutes, wait 30 minutes for the next imaging session.
Scan Regions	Any landmark is acceptable
Image Artifact	In non-clinical testing, the image artifact caused by the Nalu Neurostimulation System extends approximately 10 mm from this implant when imaged using a gradient echo pulse sequence and a 3 T MRI system.



**Important Note:** An MRI examination performed outside these guidelines may cause the electromagnetic fields used with MRI technology to interact adversely with an implanted Nalu Neurostimulation System potentially injuring the patient and/or damaging the device. Due to the risks of using MRI in a patient with an active implanted device, it is important to read, understand, and comply with all instructions to prevent potential harm or injury to the patient and/or damage to the device.

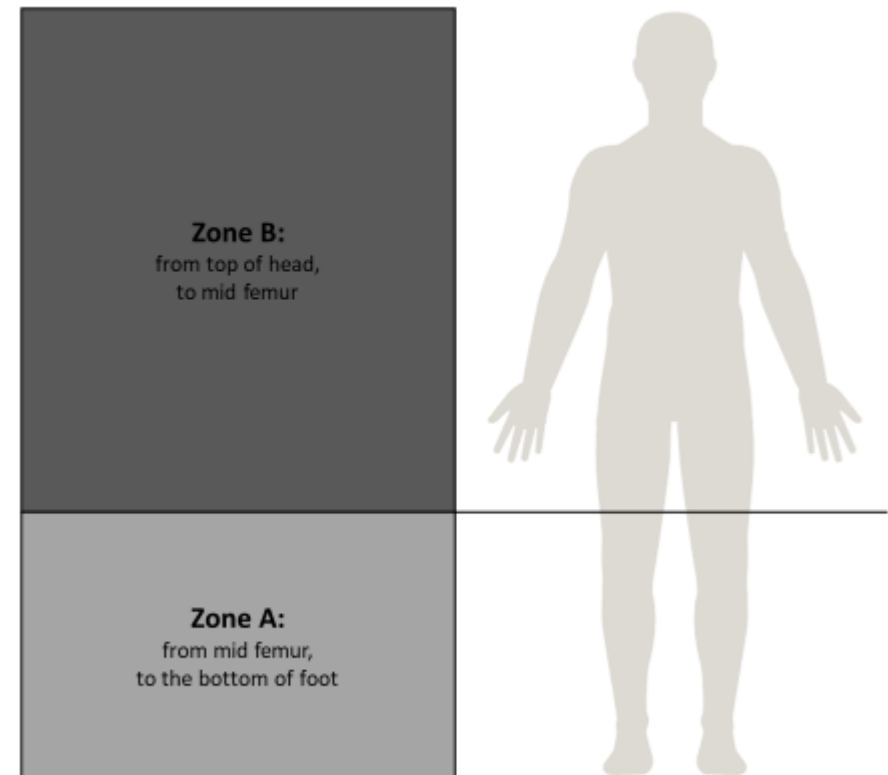

**Figure 123**

## APPENDIX A

### Whole-Body MRI Quick Reference Guide

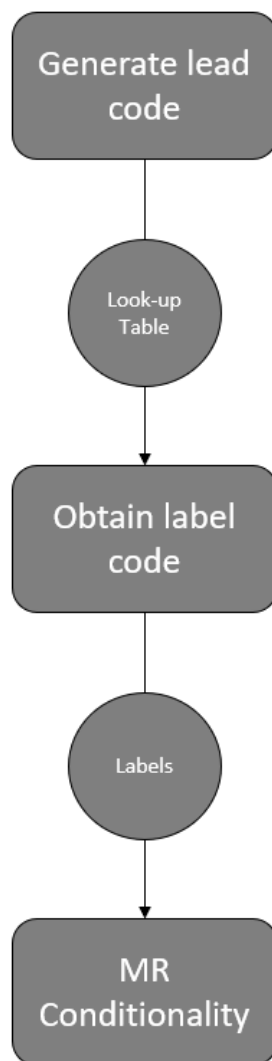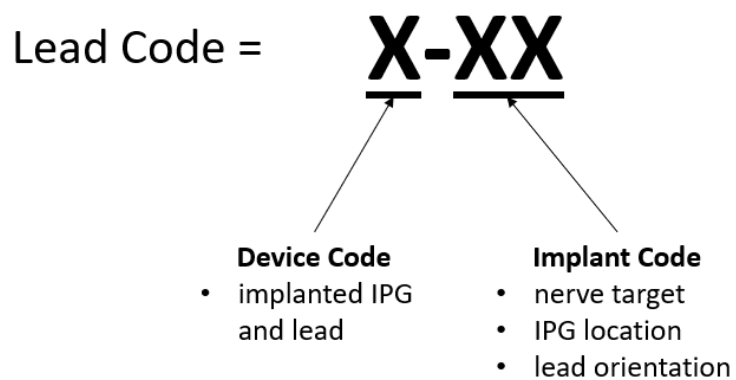

## CONTACT INFORMATION



Nalu Medical, Inc.  
2320 Faraday Ave Ste 100  
Carlsbad, CA 92008 USA  
Telephone: +1-800-618-3402  
Customer Service: [info@nalumed.com](mailto:info@nalumed.com)  
Technical Support: [support@nalumed.com](mailto:support@nalumed.com)  
[www.nalumed.com](http://www.nalumed.com)



This product can expose you to chemicals including ethylene oxide, which is known to the State of California to cause cancer and birth defects or other reproductive harm. For more information, go to [www.P65Warnings.ca.gov](http://www.P65Warnings.ca.gov).

Caution: Federal law restricts this device to sale by or on the order of a physician

**R<sub>x</sub> Only**

Nalu is a trademark of Nalu Medical Inc. Bluetooth is a registered trademark of Bluetooth® sig, Inc.